

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032237.D
 Acq On : 04 Oct 2023 18:17
 Operator : SY/MD
 Sample : 04741-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	54556	58467	14.87%	1.789%
2	1.532	146	153	168	rVB	48018	55055	14.01%	1.684%
3	2.060	307	317	331	rBV	84588	122681	31.21%	3.754%
4	3.809	852	861	896	rBV	45281	155972	39.68%	4.772%
5	4.256	984	1000	1033	rBV3	63954	197524	50.25%	6.043%
6	4.960	1200	1219	1244	rBV2	140085	361330	91.93%	11.055%
7	5.538	1388	1399	1421	rBV	101591	214395	54.54%	6.560%
8	5.834	1482	1491	1505	rVB8	3791	8490	2.16%	0.260%
9	5.995	1525	1541	1577	rBV	81413	181948	46.29%	5.567%
10	6.439	1667	1679	1700	rBV	30277	62540	15.91%	1.913%
11	6.921	1818	1829	1860	rBV2	36631	76203	19.39%	2.332%
12	7.249	1920	1931	1957	rBV	160729	296350	75.40%	9.067%
13	7.561	2020	2028	2055	rBV	21749	42863	10.90%	1.311%
14	7.911	2126	2137	2159	rVB	47247	83721	21.30%	2.562%
15	8.030	2165	2174	2208	rBV	185276	393063	100.00%	12.026%
16	8.181	2211	2221	2235	rVB	29606	53530	13.62%	1.638%
17	8.789	2399	2410	2437	rBV	158854	275908	70.19%	8.442%
18	9.673	2675	2685	2699	rVB3	6122	10687	2.72%	0.327%
19	10.159	2824	2836	2852	rBV	60960	97477	24.80%	2.982%
20	11.191	3142	3157	3176	rBV	167064	262601	66.81%	8.035%
21	11.564	3262	3273	3290	rBV	163696	257585	65.53%	7.881%




Sum of corrected areas: 3268390

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032237.D
Acq On : 04 Oct 2023 18:17
Operator : SY/MD
Sample : 04741-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

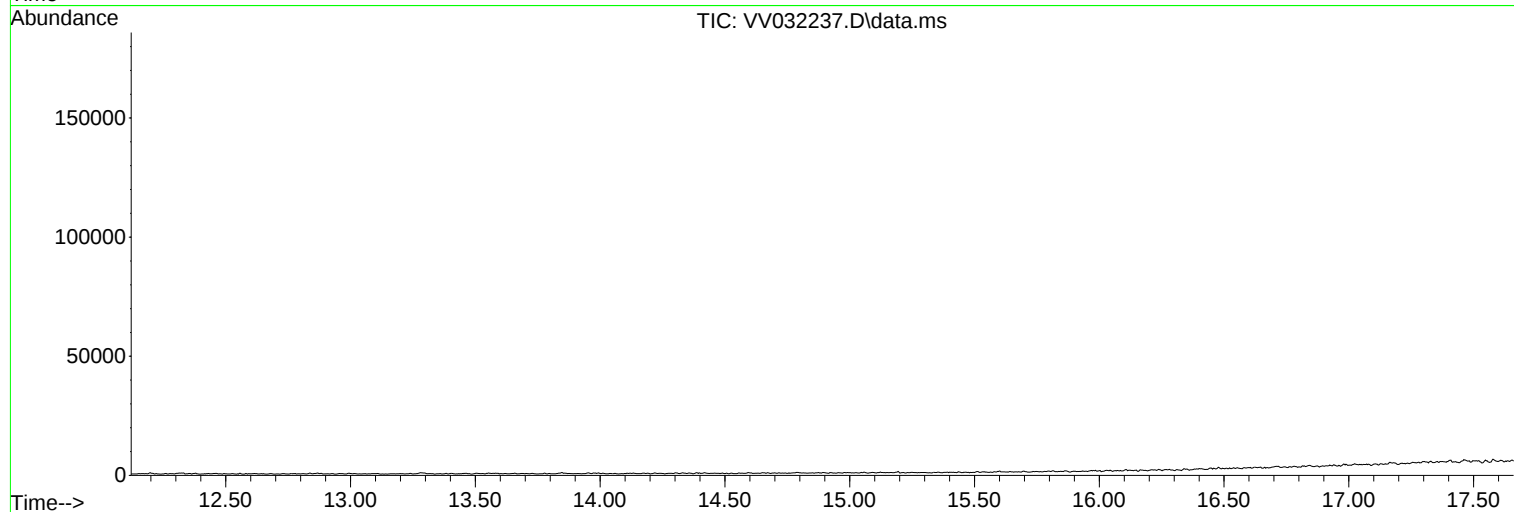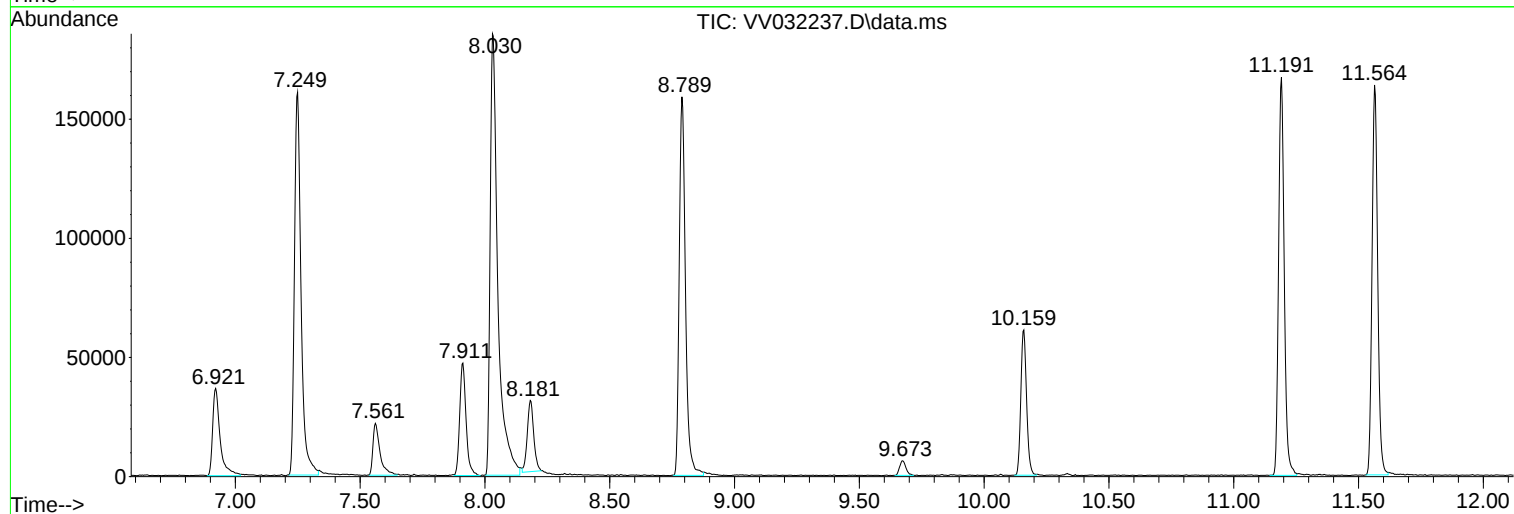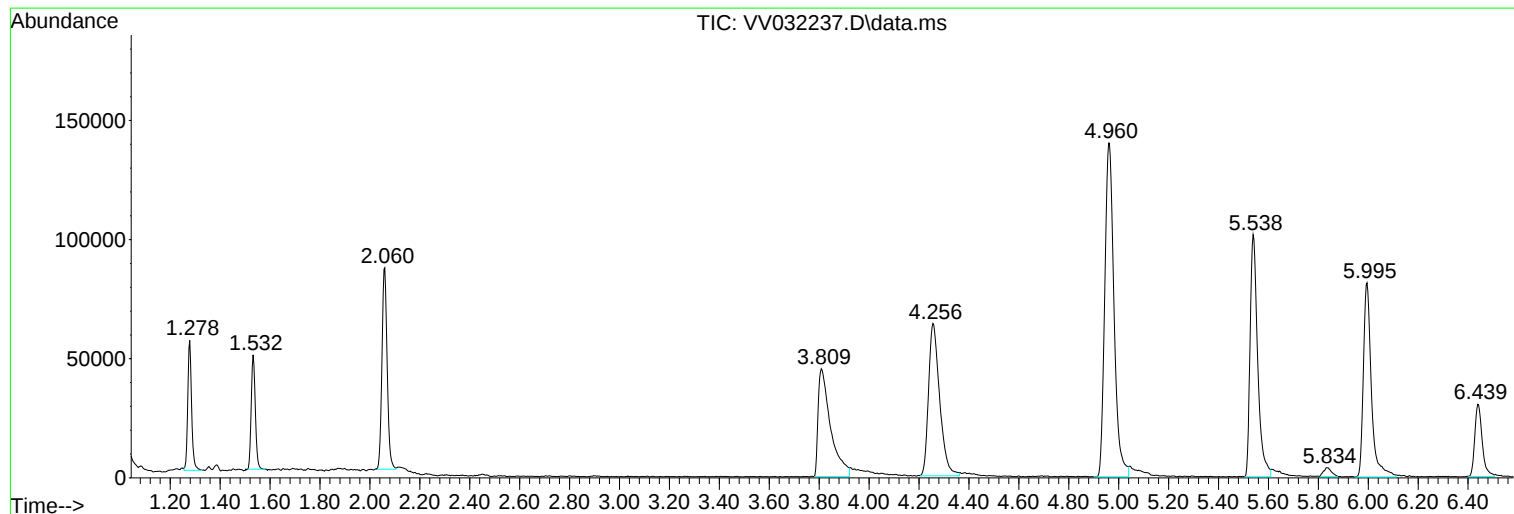

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032237.D
Acq On : 04 Oct 2023 18:17
Operator : SY/MD
Sample : 04741-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032237.D
Acq On : 04 Oct 2023 18:17
Operator : SY/MD
Sample : 04741-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc