

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032238.D
 Acq On : 04 Oct 2023 18:42
 Operator : SY/MD
 Sample : 04741-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032238.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	55366	57052	14.35%	1.726%
2	1.532	145	153	170	rVB	50343	59231	14.90%	1.792%
3	2.060	307	317	333	rBV	87580	127187	31.99%	3.847%
4	3.802	850	859	900	rBV	50711	155877	39.20%	4.715%
5	4.256	983	1000	1031	rBV3	63372	198773	49.99%	6.012%
6	4.963	1203	1220	1247	rBV2	141571	368025	92.55%	11.132%
7	5.539	1387	1399	1425	rBV	99897	215716	54.25%	6.525%
8	5.834	1482	1491	1502	rBV6	4192	8763	2.20%	0.265%
9	5.995	1528	1541	1569	rBV	81984	181015	45.52%	5.475%
10	6.439	1667	1679	1699	rBV	31252	63328	15.93%	1.916%
11	6.921	1819	1829	1859	rBV	37505	76738	19.30%	2.321%
12	7.249	1918	1931	1961	rBV	162589	301924	75.93%	9.133%
13	7.561	2019	2028	2044	rBV	21701	40489	10.18%	1.225%
14	7.912	2125	2137	2159	rVB2	49303	88490	22.25%	2.677%
15	8.031	2163	2174	2210	rBV	189284	397643	100.00%	12.028%
16	8.182	2211	2221	2243	rVB2	30594	58030	14.59%	1.755%
17	8.789	2399	2410	2436	rBV	158579	274657	69.07%	8.308%
18	9.674	2674	2685	2699	rBV2	6479	10578	2.66%	0.320%
19	10.159	2820	2836	2850	rBV	60993	99791	25.10%	3.018%
20	11.191	3144	3157	3182	rBV	163216	262691	66.06%	7.946%
21	11.564	3262	3273	3293	rBV	168062	260017	65.39%	7.865%




Sum of corrected areas: 3306015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032238.D
Acq On : 04 Oct 2023 18:42
Operator : SY/MD
Sample : 04741-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

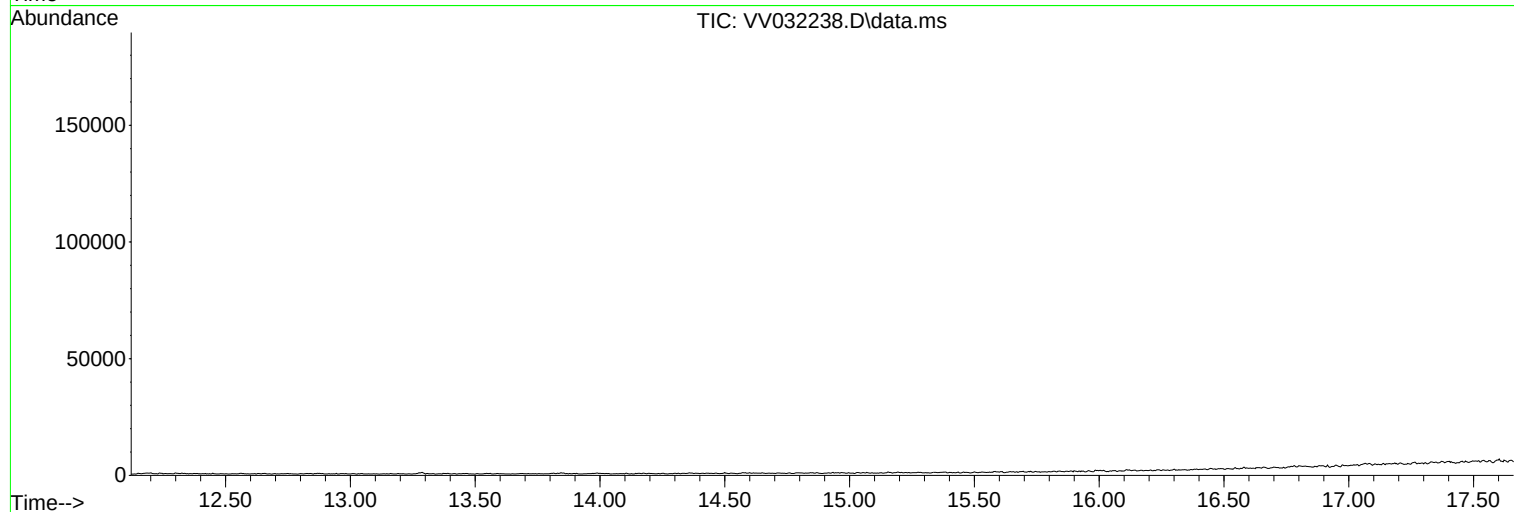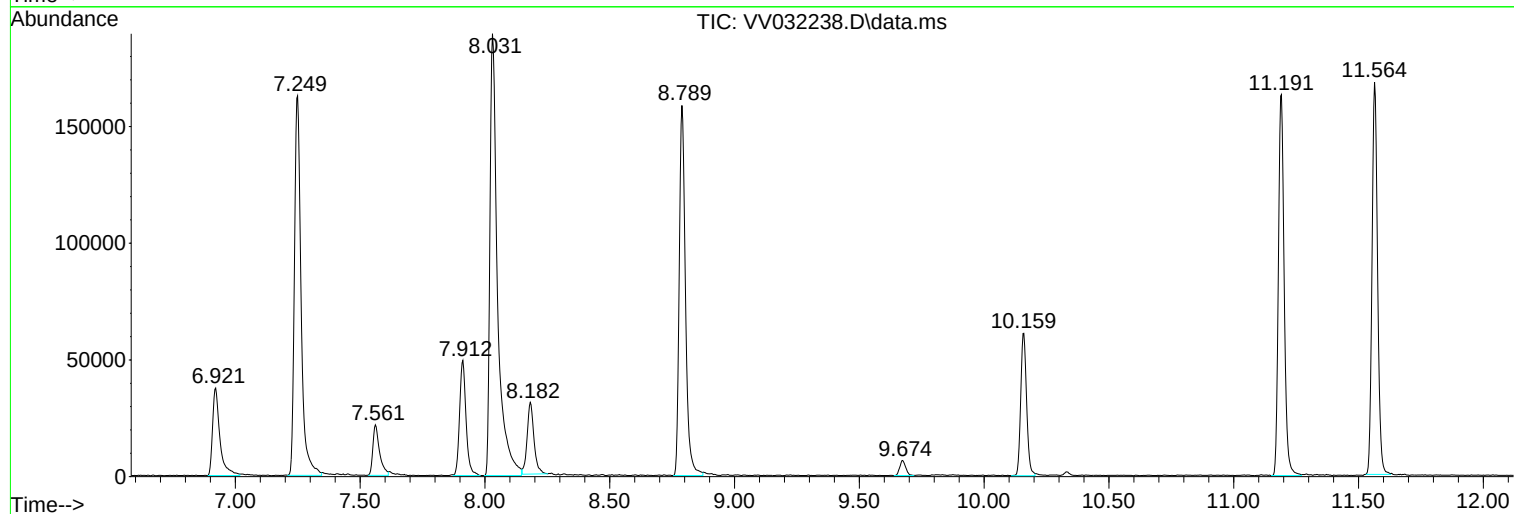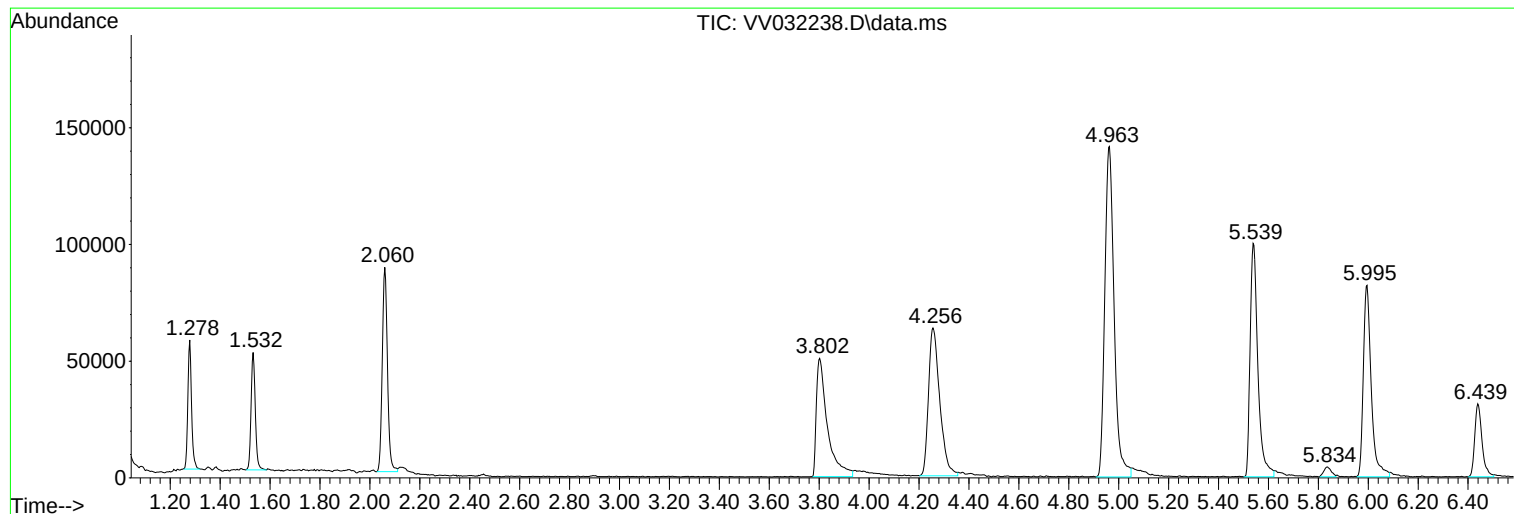

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032238.D
Acq On : 04 Oct 2023 18:42
Operator : SY/MD
Sample : 04741-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032238.D
Acq On : 04 Oct 2023 18:42
Operator : SY/MD
Sample : 04741-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------