

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032239.D
 Acq On : 04 Oct 2023 19:06
 Operator : SY/MD
 Sample : 04741-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	53064	57208	14.19%	1.832%
2	1.532	145	153	168	rVB	49668	58329	14.47%	1.868%
3	2.056	306	316	334	rBV	84669	126370	31.34%	4.047%
4	3.818	851	864	893	rBV	40604	148541	36.84%	4.757%
5	4.252	981	999	1025	rBV2	60066	158467	39.30%	5.075%
6	4.960	1205	1219	1245	rBV2	142859	366176	90.81%	11.728%
7	5.539	1386	1399	1425	rBV	103604	223763	55.49%	7.167%
8	5.834	1481	1491	1505	rVB5	3758	7865	1.95%	0.252%
9	5.992	1528	1540	1583	rBV	81468	185885	46.10%	5.953%
10	6.445	1672	1681	1692	rBV5	2406	4493	1.11%	0.144%
11	6.921	1819	1829	1849	rBV	36484	72883	18.07%	2.334%
12	7.249	1919	1931	1955	rBV	160321	298794	74.10%	9.570%
13	7.561	2017	2028	2054	rBV2	21543	43524	10.79%	1.394%
14	7.911	2128	2137	2158	rVB2	20945	36518	9.06%	1.170%
15	8.034	2165	2175	2213	rBV	186554	403242	100.00%	12.915%
16	8.185	2214	2222	2233	rVB3	5883	11947	2.96%	0.383%
17	8.789	2400	2410	2431	rBV	163766	281737	69.87%	9.023%
18	10.159	2824	2836	2863	rBV	61194	100499	24.92%	3.219%
19	11.191	3146	3157	3180	rBV	171526	273686	67.87%	8.766%
20	11.564	3263	3273	3295	rBV	163082	262380	65.07%	8.403%




Sum of corrected areas: 3122307

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032239.D
Acq On : 04 Oct 2023 19:06
Operator : SY/MD
Sample : 04741-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

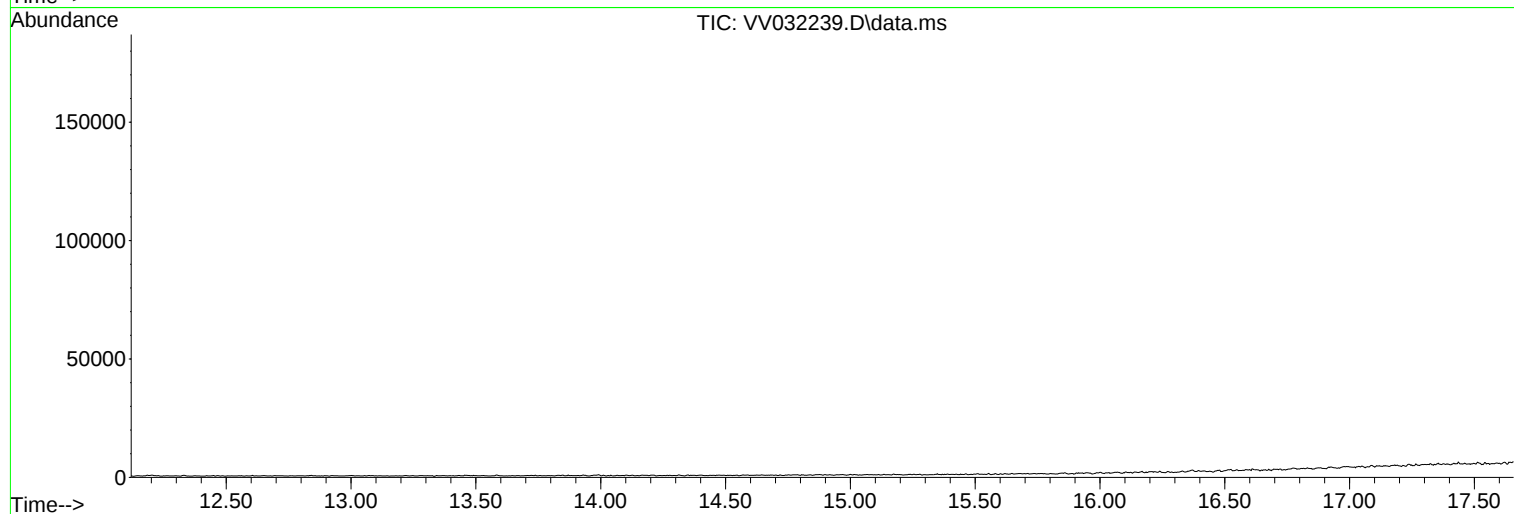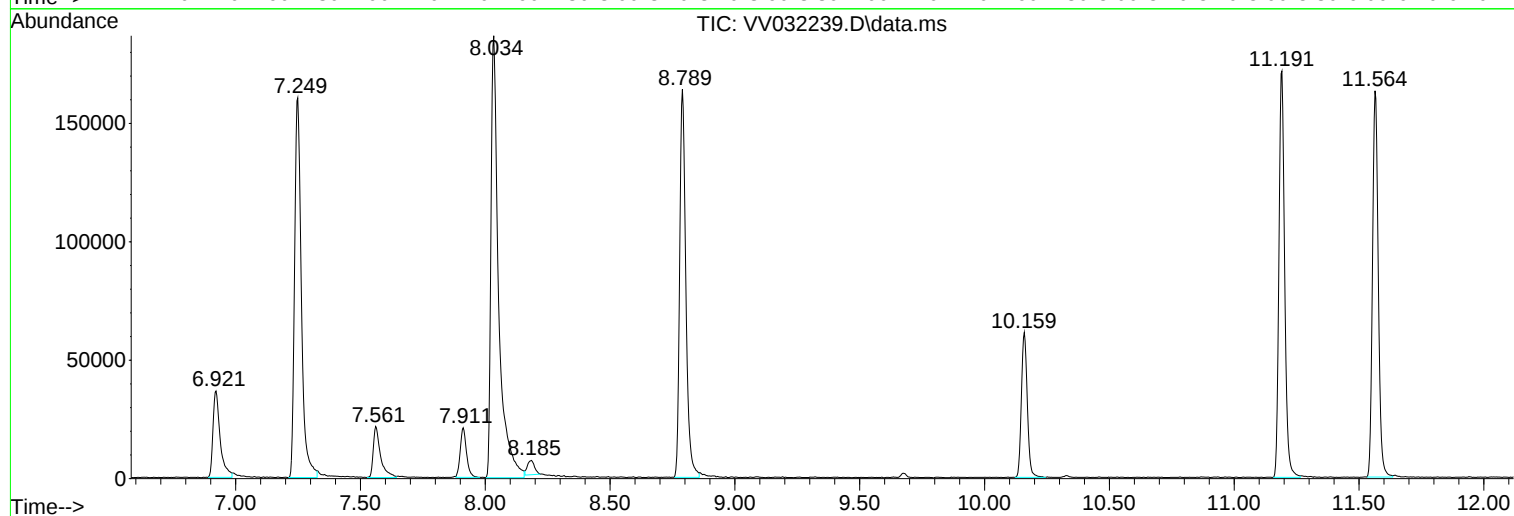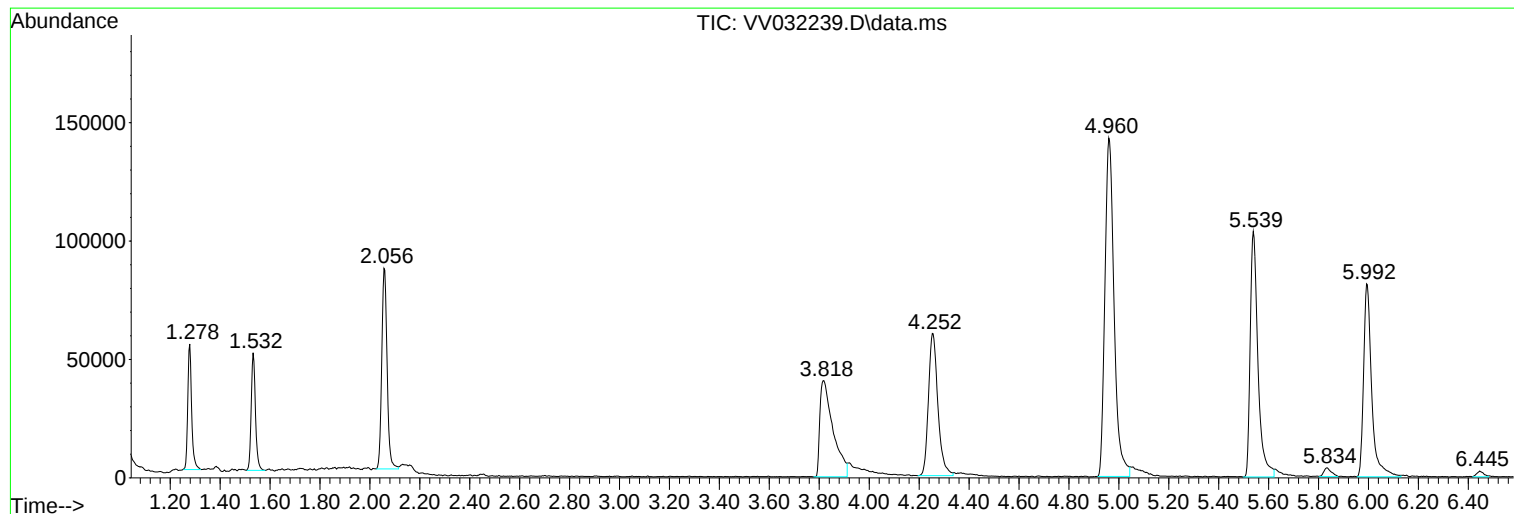

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032239.D
Acq On : 04 Oct 2023 19:06
Operator : SY/MD
Sample : 04741-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032239.D
Acq On : 04 Oct 2023 19:06
Operator : SY/MD
Sample : 04741-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc