

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
 Data File : VV032241.D
 Acq On : 04 Oct 2023 19:56
 Operator : SY/MD
 Sample : 04708-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJT3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	8	14	30	rVB	167769	160352	4.03%	2.134%
2	1.278	65	74	87	rBV3	110427	138646	3.49%	1.845%
3	1.532	144	153	164	rBV	53455	63545	1.60%	0.846%
4	2.059	307	317	331	rBV	87542	128170	3.22%	1.706%
5	3.799	847	858	895	rBV	51487	154037	3.87%	2.050%
6	4.275	984	1006	1029	rBV4	116176	403688	10.15%	5.372%
7	4.963	1204	1220	1253	rBV2	141965	376978	9.48%	5.017%
8	5.538	1388	1399	1423	rBV	97455	209107	5.26%	2.783%
9	5.834	1476	1491	1530	rBV	1980512	3975526	100.00%	52.905%
10	5.992	1530	1540	1563	rVB	84958	181999	4.58%	2.422%
11	6.921	1817	1829	1856	rBV	37099	77716	1.95%	1.034%
12	7.246	1919	1930	1950	rBV	163171	301364	7.58%	4.010%
13	7.561	2019	2028	2043	rBV	22369	42284	1.06%	0.563%
14	8.030	2164	2174	2215	rBV	193602	409442	10.30%	5.449%
15	8.789	2400	2410	2434	rBV	157934	267857	6.74%	3.565%
16	10.159	2825	2836	2860	rBV	62800	102230	2.57%	1.360%
17	11.188	3146	3156	3177	rBV	164885	259624	6.53%	3.455%
18	11.564	3263	3273	3289	rVB	166401	261924	6.59%	3.486%




Sum of corrected areas: 7514489

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032241.D
Acq On : 04 Oct 2023 19:56
Operator : SY/MD
Sample : 04708-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

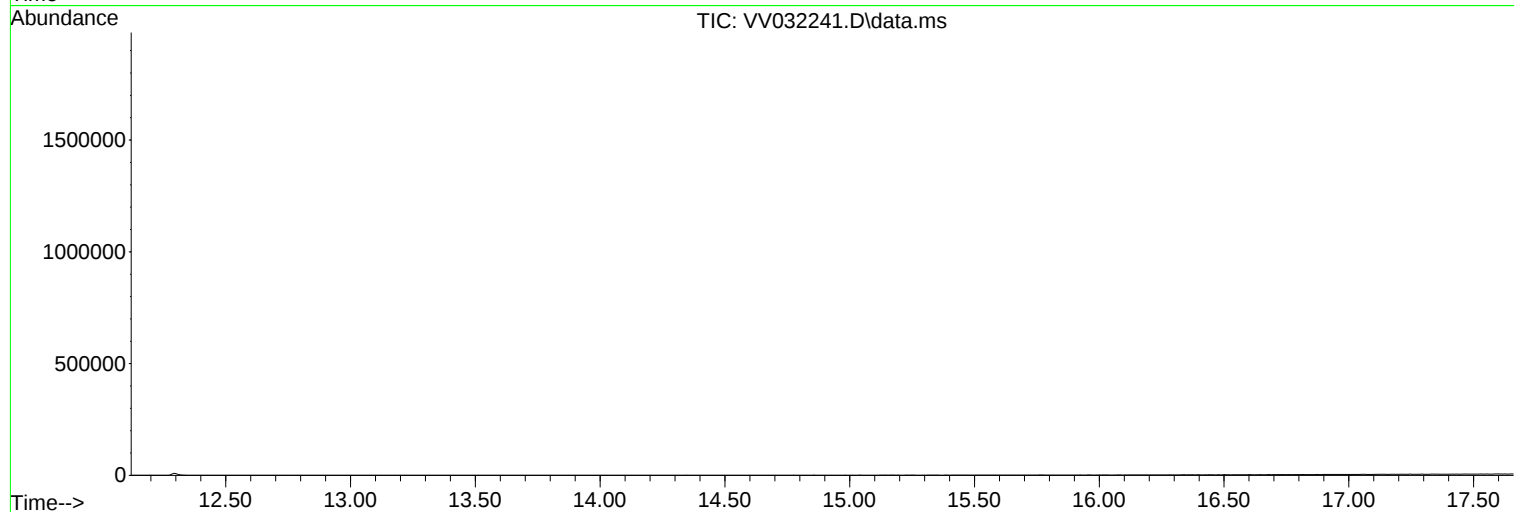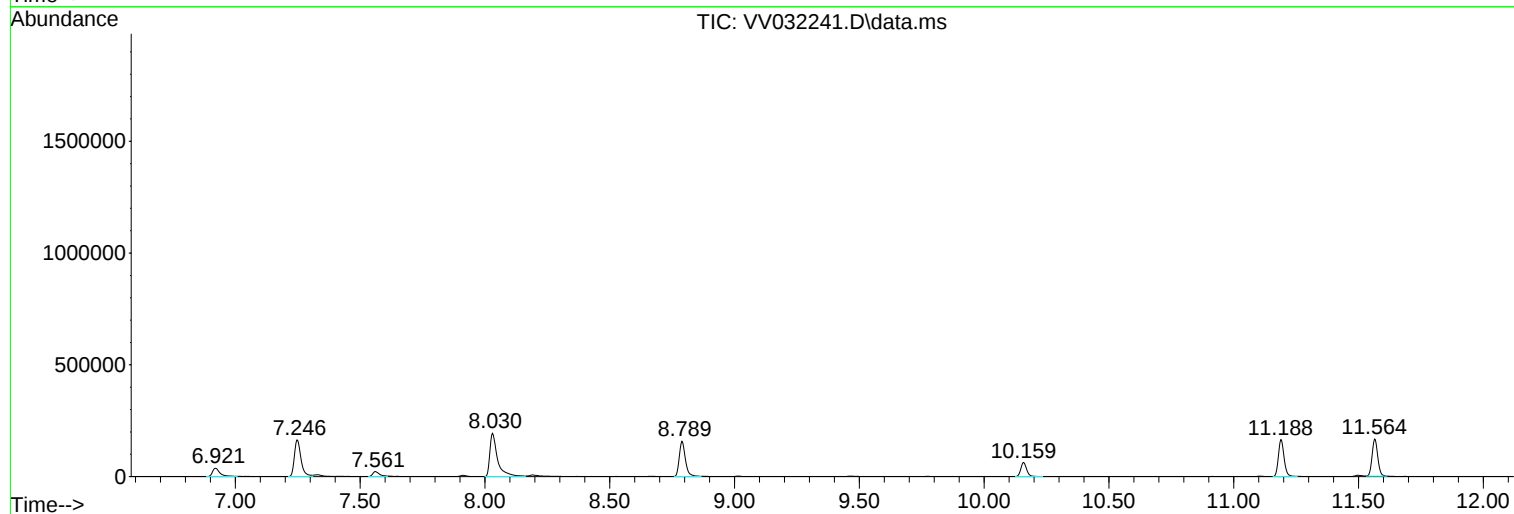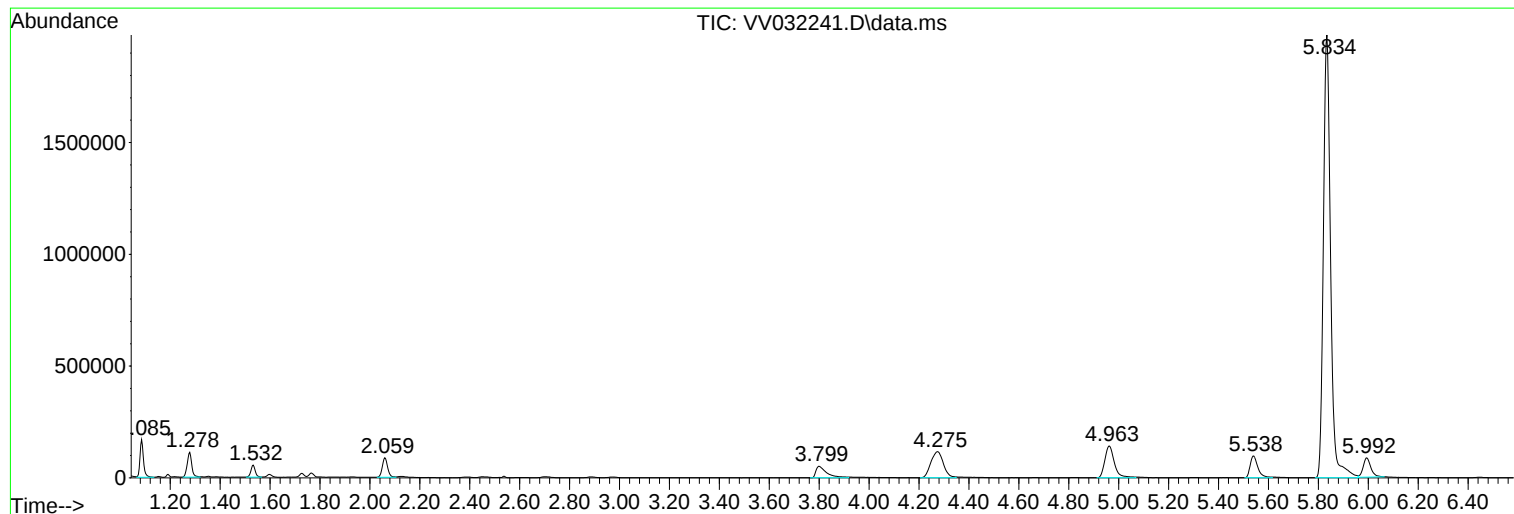

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032241.D
Acq On : 04 Oct 2023 19:56
Operator : SY/MD
Sample : 04708-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJT3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.085	3.83 ug/L	160352	1,4-Difluorobenzene	5.542

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	90
2			Propene	42	C3H6	000115-07-1	42
3			Cyclopropane	42	C3H6	000075-19-4	9
4			Cyclopropane	42	C3H6	000075-19-4	7
5			Cyclopropene	40	C3H4	002781-85-3	5

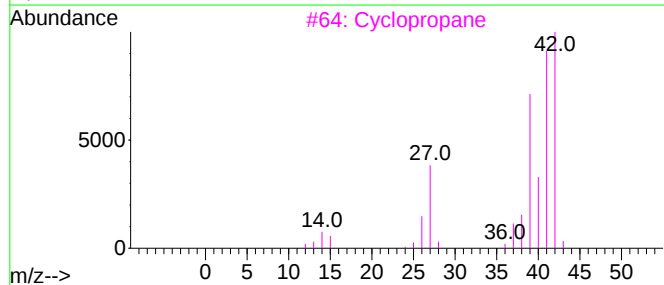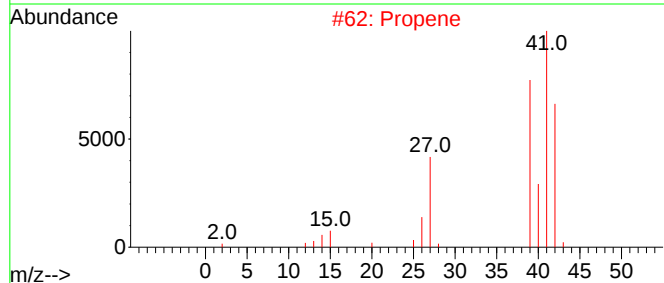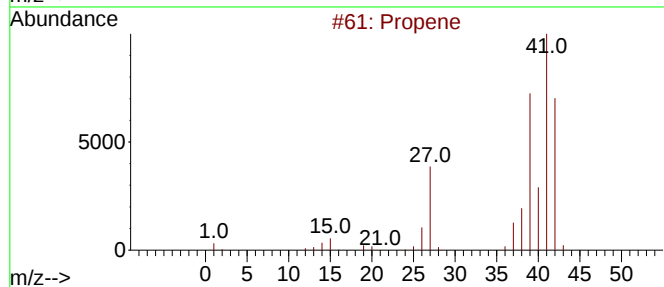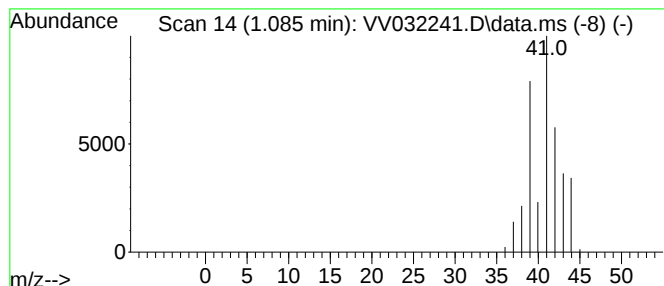

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032241.D
Acq On : 04 Oct 2023 19:56
Operator : SY/MD
Sample : 04708-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.085	3.8	ug/L	160352	1	5.542	209107	5.0