


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100423\
Data File : VV032216.D
Acq On : 04 Oct 2023 08:41
Operator : SY/MD
Sample : BFB214
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB214

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 05 01:37:52 2023

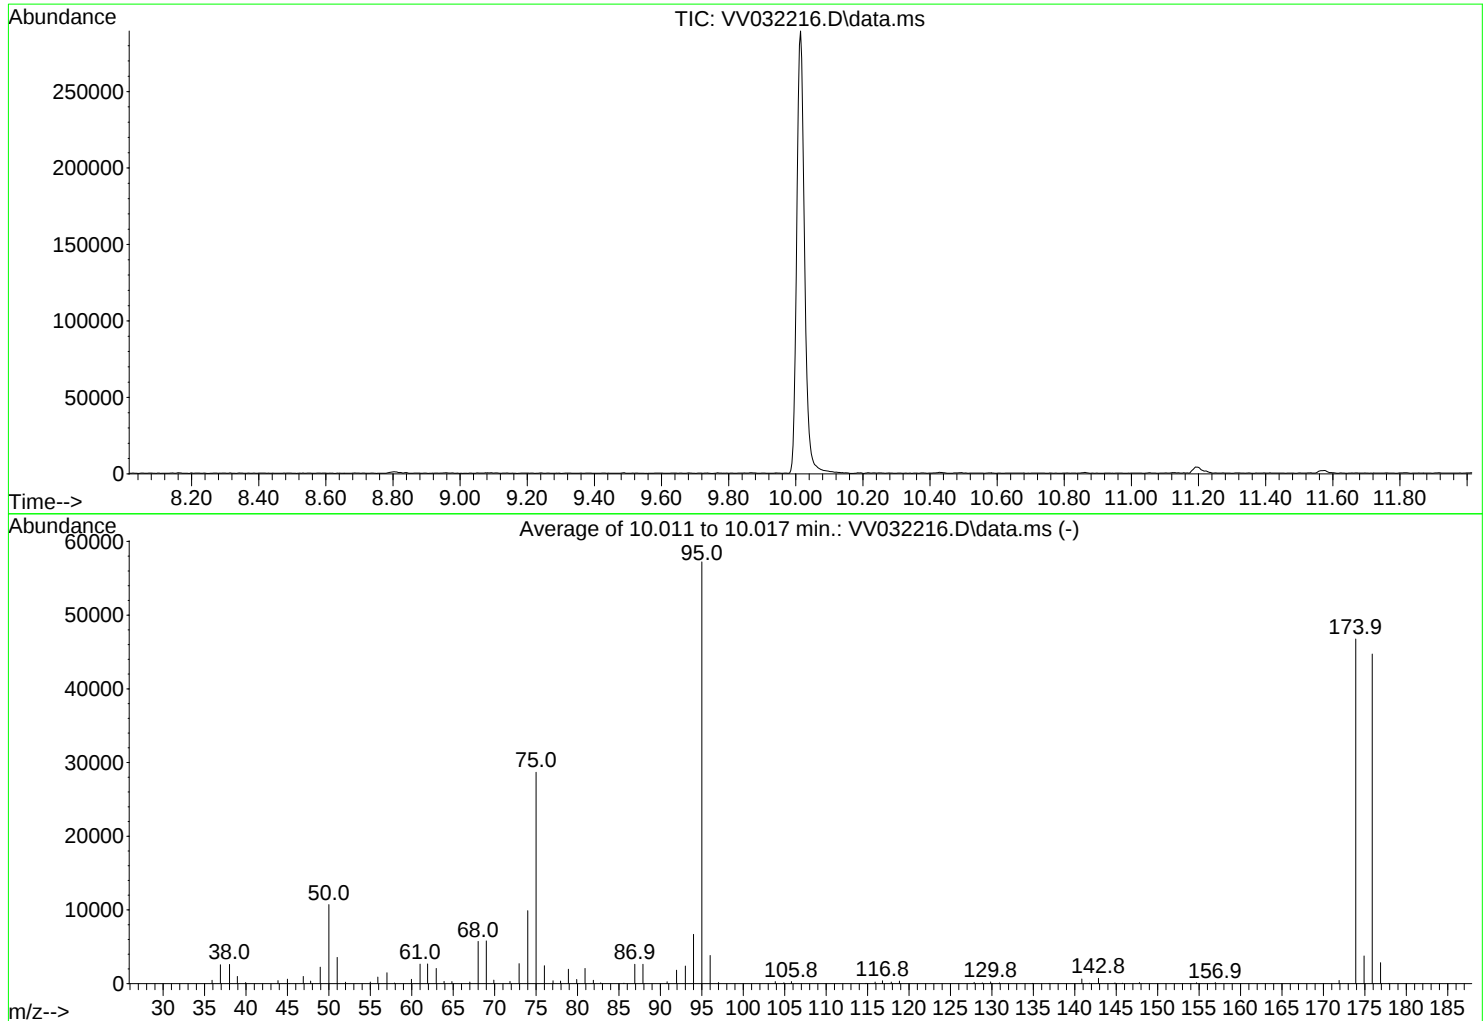

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	10730	PASS
75	95	30	80	50.1	28677	PASS
95	95	100	100	100.0	57232	PASS
96	95	5	9	6.7	3825	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.7	46771	PASS
175	174	5	9	8.0	3764	PASS
176	174	95	105	95.6	44723	PASS
177	176	5	10	6.3	2835	PASS

m/z	Abundance
39.70	138.0
43.00	100.0
43.80	332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.90	457.0
36.90	2680.0
38.00	2634.0
39.00	1039.0
40.00	144.0
43.90	786.0
45.00	607.0
46.90	957.0
47.80	382.0
48.90	2319.0
50.00	11103.0
51.00	3770.0
52.00	232.0
55.00	206.0
55.90	874.0
57.00	1577.0
60.00	576.0
61.00	2693.0
61.90	2716.0
62.90	2154.0
63.90	324.0
64.90	232.0
67.00	235.0
68.00	5652.0
69.00	5897.0
69.90	488.0
71.80	293.0
72.90	2677.0
74.00	9889.0
75.00	28880.0
76.00	2425.0
77.00	424.0
78.00	354.0
78.90	1922.0
79.90	565.0
80.90	2151.0
81.90	466.0
82.80	116.0
85.60	114.0
86.90	2643.0
87.90	2670.0
90.80	244.0
91.90	1763.0
93.00	2389.0
94.00	6575.0
95.00	58224.0
96.00	3941.0
97.00	168.0
103.80	251.0
104.90	143.0
105.80	260.0
114.80	121.0
115.90	249.0
116.80	397.0
117.90	214.0
118.90	365.0
127.90	152.0
128.90	137.0
129.80	234.0
130.90	133.0
136.90	106.0
140.90	580.0
141.80	110.0
142.80	709.0
144.90	101.0
147.80	149.0
154.70	138.0
156.90	157.0
171.90	441.0
173.90	45832.0
174.90	3740.0
175.90	43264.0
176.90	2824.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.90	463.0
36.90	2612.0
38.00	2696.0
38.90	1000.0
40.00	156.0
43.90	772.0
45.00	627.0
46.90	1005.0
47.80	362.0
48.90	2294.0
50.00	11028.0
51.00	3666.0
52.00	208.0
55.00	229.0
55.90	901.0
57.00	1521.0
57.90	126.0
60.00	636.0
61.00	2720.0
61.90	2756.0
62.90	2131.0
63.90	306.0
64.80	282.0
67.00	235.0
68.00	5922.0
69.00	5969.0
69.90	504.0
71.80	303.0
73.00	2788.0
74.00	10153.0
75.00	29632.0
76.00	2494.0
77.00	401.0
78.00	366.0
78.90	1999.0
79.90	600.0
80.90	2126.0
81.90	480.0
82.80	122.0
85.60	109.0
86.90	2729.0
87.90	2689.0
90.80	273.0
92.00	1911.0
93.00	2468.0
94.00	6892.0
95.00	59000.0
96.00	3904.0
97.00	169.0
103.90	293.0
104.90	127.0
105.80	294.0
115.90	235.0
116.80	402.0
117.90	235.0
118.90	363.0
127.80	182.0
128.90	122.0
129.90	242.0
130.90	121.0
140.90	652.0
141.80	102.0
142.90	746.0
144.80	108.0
145.70	108.0
147.80	153.0
154.70	141.0
157.00	162.0
171.90	462.0
173.90	48288.0
174.90	3926.0
175.90	46456.0
176.90	2936.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
35.90	464.0
36.90	2376.0
38.00	2521.0
39.00	912.0
39.90	167.0
43.90	702.0
45.00	578.0
46.90	979.0
47.80	309.0
49.00	2114.0
50.00	10058.0
51.00	3251.0
52.00	154.0
55.00	240.0
55.90	865.0
57.00	1341.0
57.90	136.0
59.90	554.0
61.00	2551.0
61.90	2524.0
63.00	1921.0
63.90	266.0
64.90	313.0
67.00	212.0
68.00	5613.0
69.00	5500.0
69.90	473.0
71.90	299.0
73.00	2679.0
74.00	9651.0
75.00	27520.0
76.00	2391.0
77.10	331.0
77.90	324.0
78.90	1918.0
79.90	567.0
80.90	1926.0
81.90	444.0
82.80	117.0
86.90	2539.0
87.90	2533.0
90.80	287.0
92.00	1802.0
93.00	2293.0
94.00	6618.0
95.00	54472.0
96.00	3629.0
97.00	145.0
103.90	319.0
104.90	108.0
105.80	312.0
115.90	202.0
116.80	403.0
117.80	220.0
118.80	336.0
127.80	208.0
128.80	103.0
129.80	227.0
130.90	108.0
134.90	102.0
140.80	669.0
142.90	718.0
144.80	116.0
145.80	120.0
147.80	151.0
154.70	142.0
157.00	140.0
171.90	389.0
173.90	46192.0
174.90	3627.0
175.90	44448.0
176.90	2744.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214