

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008107.D
 Acq On : 05 Oct 2018 19:31
 Operator : SY/MD
 Sample : J5278-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYD9

Quant Time: Oct 06 02:00:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 01:03:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	102657	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	98193	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	44751	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	26516	4.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.20%
7) Chloroethane-d5	1.59	69	23181	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.20%
11) 1,1-Dichloroethene-d2	2.14	63	40722	3.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.00%
20) 2-Butanone-d5	3.96	46	70531	46.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.04%
24) Chloroform-d	4.41	84	57583	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.09	65	29675	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
32) Benzene-d6	5.10	84	111438	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
36) 1,2-Dichloropropane-d6	6.12	67	34546	4.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.80%
41) Toluene-d8	7.36	98	98711	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.00%
43) trans-1,3-Dichloropropene-	7.67	79	11368	4.10	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.00%
46) 2-Hexanone-d5	8.14	63	46608	42.21	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.42%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	23637	4.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	39806	4.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	2060	2.006 ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008107.D
Acq On : 05 Oct 2018 19:31
Operator : SY/MD
Sample : J5278-02
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYD9

Quant Time: Oct 06 02:00:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 01:03:16 2018
Response via : Initial Calibration

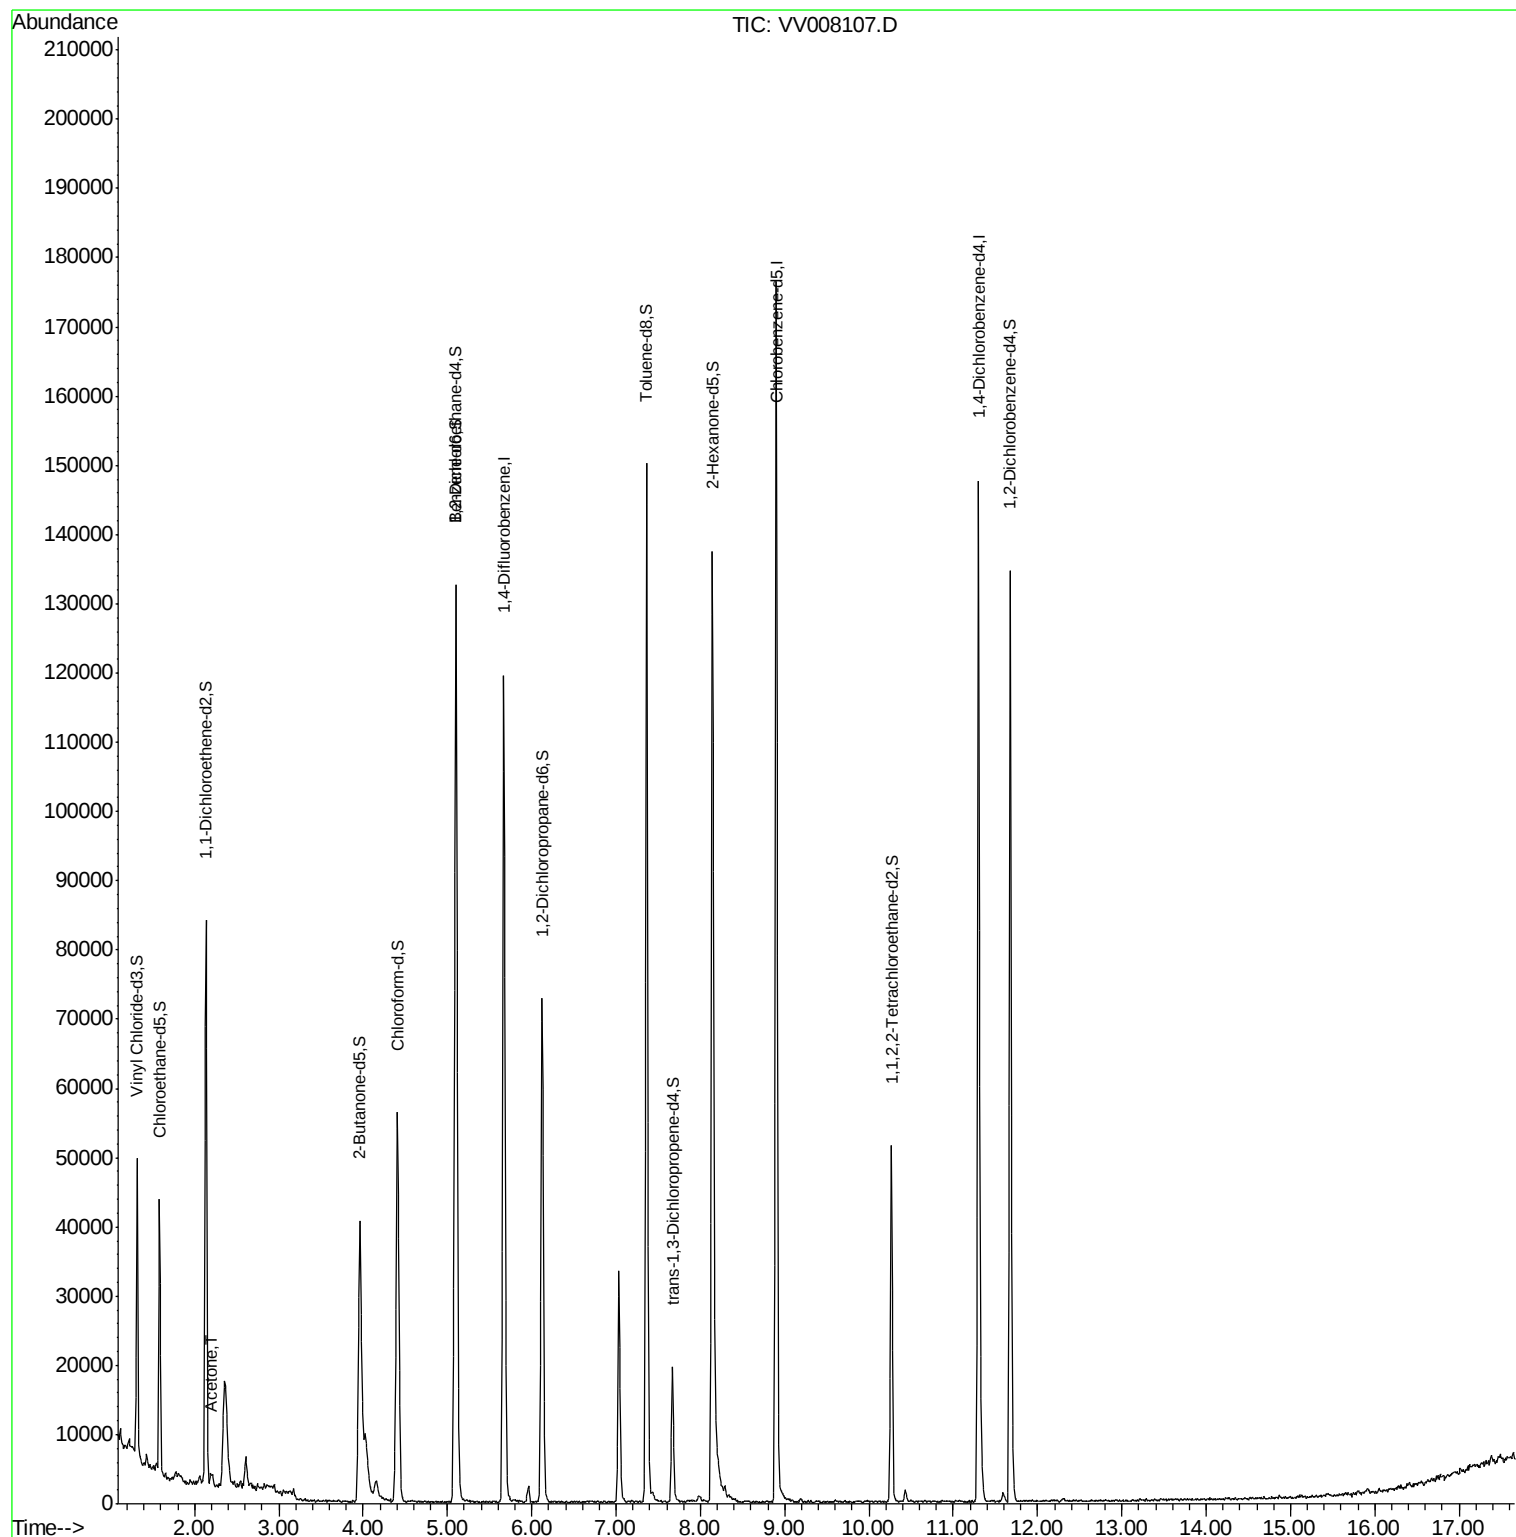

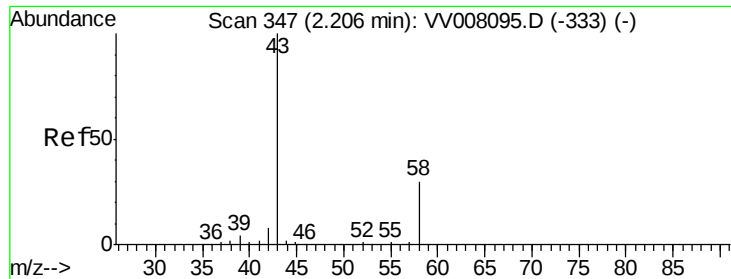

#13

Acetone

Concen: 2.006 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.00 min

Lab File: VV008107.D

Acq: 05 Oct 2018 19:31


Instrument :
MSVOA_V
ClientSampleId :
BEYD9

Tot Ion: 43 Resp: 2060

Ion Ratio Lower Upper



43 100

58 21.0 0.0 62.2

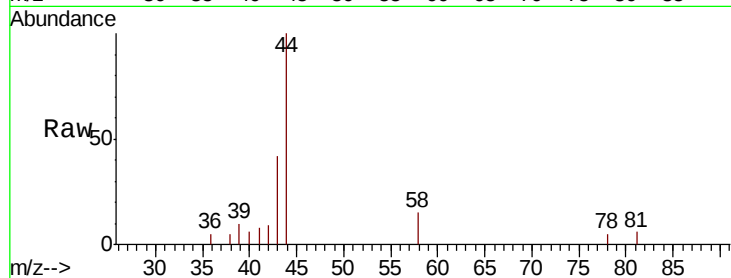

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

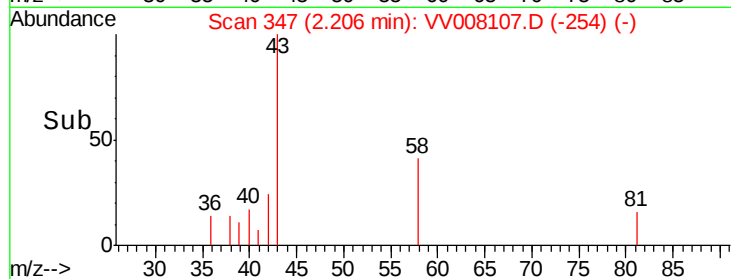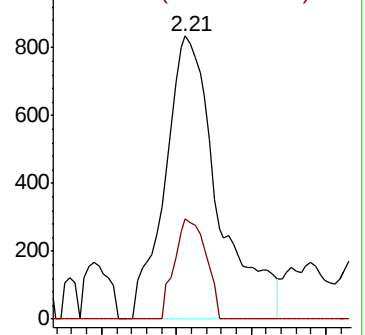

Time-->