

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008108.D
 Acq On : 05 Oct 2018 19:58
 Operator : SY/MD
 Sample : J5278-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYE0

Quant Time: Oct 06 02:03:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 01:03:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	102048	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	96790	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	44479	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27194	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	1.59	69	23097	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.14	63	41152	3.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.20%
20) 2-Butanone-d5	3.96	46	70618	46.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.72%
24) Chloroform-d	4.41	84	57836	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.09	65	29769	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
32) Benzene-d6	5.10	84	110903	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
36) 1,2-Dichloropropane-d6	6.12	67	34824	4.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.80%
41) Toluene-d8	7.36	98	99463	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	7.67	79	11275	4.13	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.60%
46) 2-Hexanone-d5	8.14	63	48369	44.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.88%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	24246	4.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	40375	4.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	2428	2.378 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008108.D
Acq On : 05 Oct 2018 19:58
Operator : SY/MD
Sample : J5278-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE0

Quant Time: Oct 06 02:03:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 01:03:16 2018
Response via : Initial Calibration

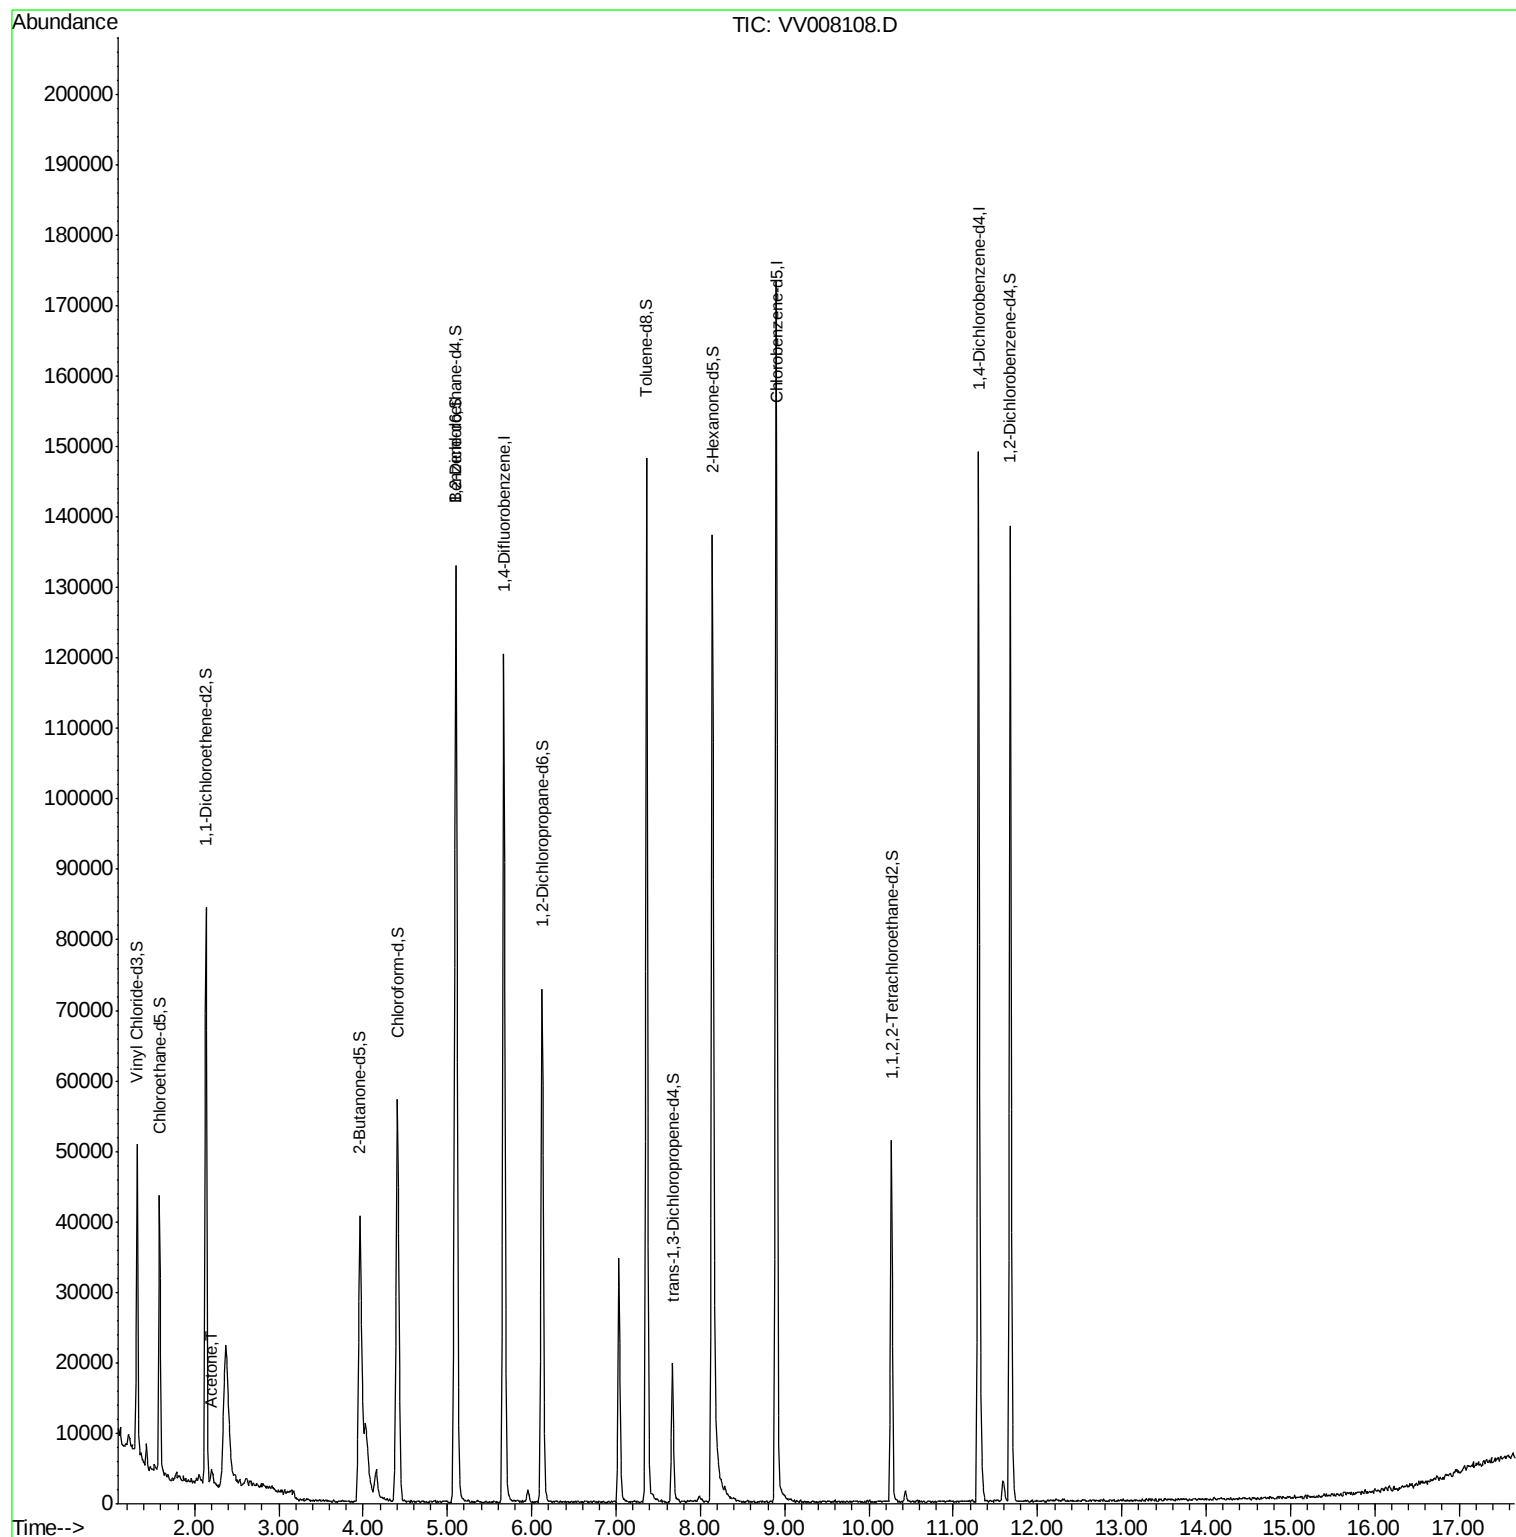

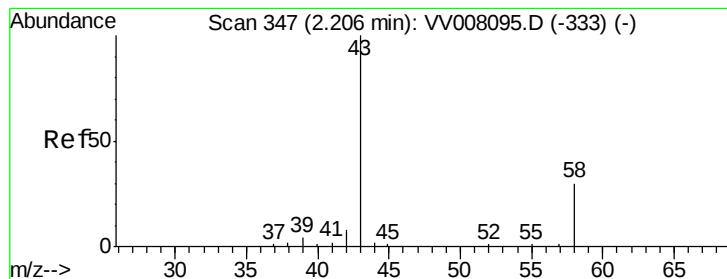

#13
 Acetone
 Concen: 2.378 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. 0.00 min
 Lab File: VV008108.D
 Acq: 05 Oct 2018 19:58

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYE0

Tot Ion: 43 Resp: 2428
 Ion Ratio Lower Upper
 43 100
 58 21.5 0.0 62.2

