

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008110.D
 Acq On : 05 Oct 2018 20:53
 Operator : SY/MD
 Sample : J5278-05
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYE2

Quant Time: Oct 06 02:14:42 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 01:03:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	102862	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	98833	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	44158	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	26102	4.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.60%
7) Chloroethane-d5	1.59	69	22777	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.60%
11) 1,1-Dichloroethene-d2	2.14	63	39893	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	3.96	46	69402	45.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.38%
24) Chloroform-d	4.41	84	55486	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.20%
26) 1,2-Dichloroethane-d4	5.09	65	28588	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
32) Benzene-d6	5.10	84	108358	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.80%
36) 1,2-Dichloropropane-d6	6.13	67	33943	4.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.80%
41) Toluene-d8	7.36	98	97512	3.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.40%
43) trans-1,3-Dichloropropene-	7.67	79	11023	3.95	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.00%
46) 2-Hexanone-d5	8.14	63	45992	41.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.76%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	23944	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	39354	4.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.00%


Target Compounds					Ovalue
25) Chloroform	4.44	83	2576	0.207 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008110.D
Acq On : 05 Oct 2018 20:53
Operator : SY/MD
Sample : J5278-05
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE2

Quant Time: Oct 06 02:14:42 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 01:03:16 2018
Response via : Initial Calibration

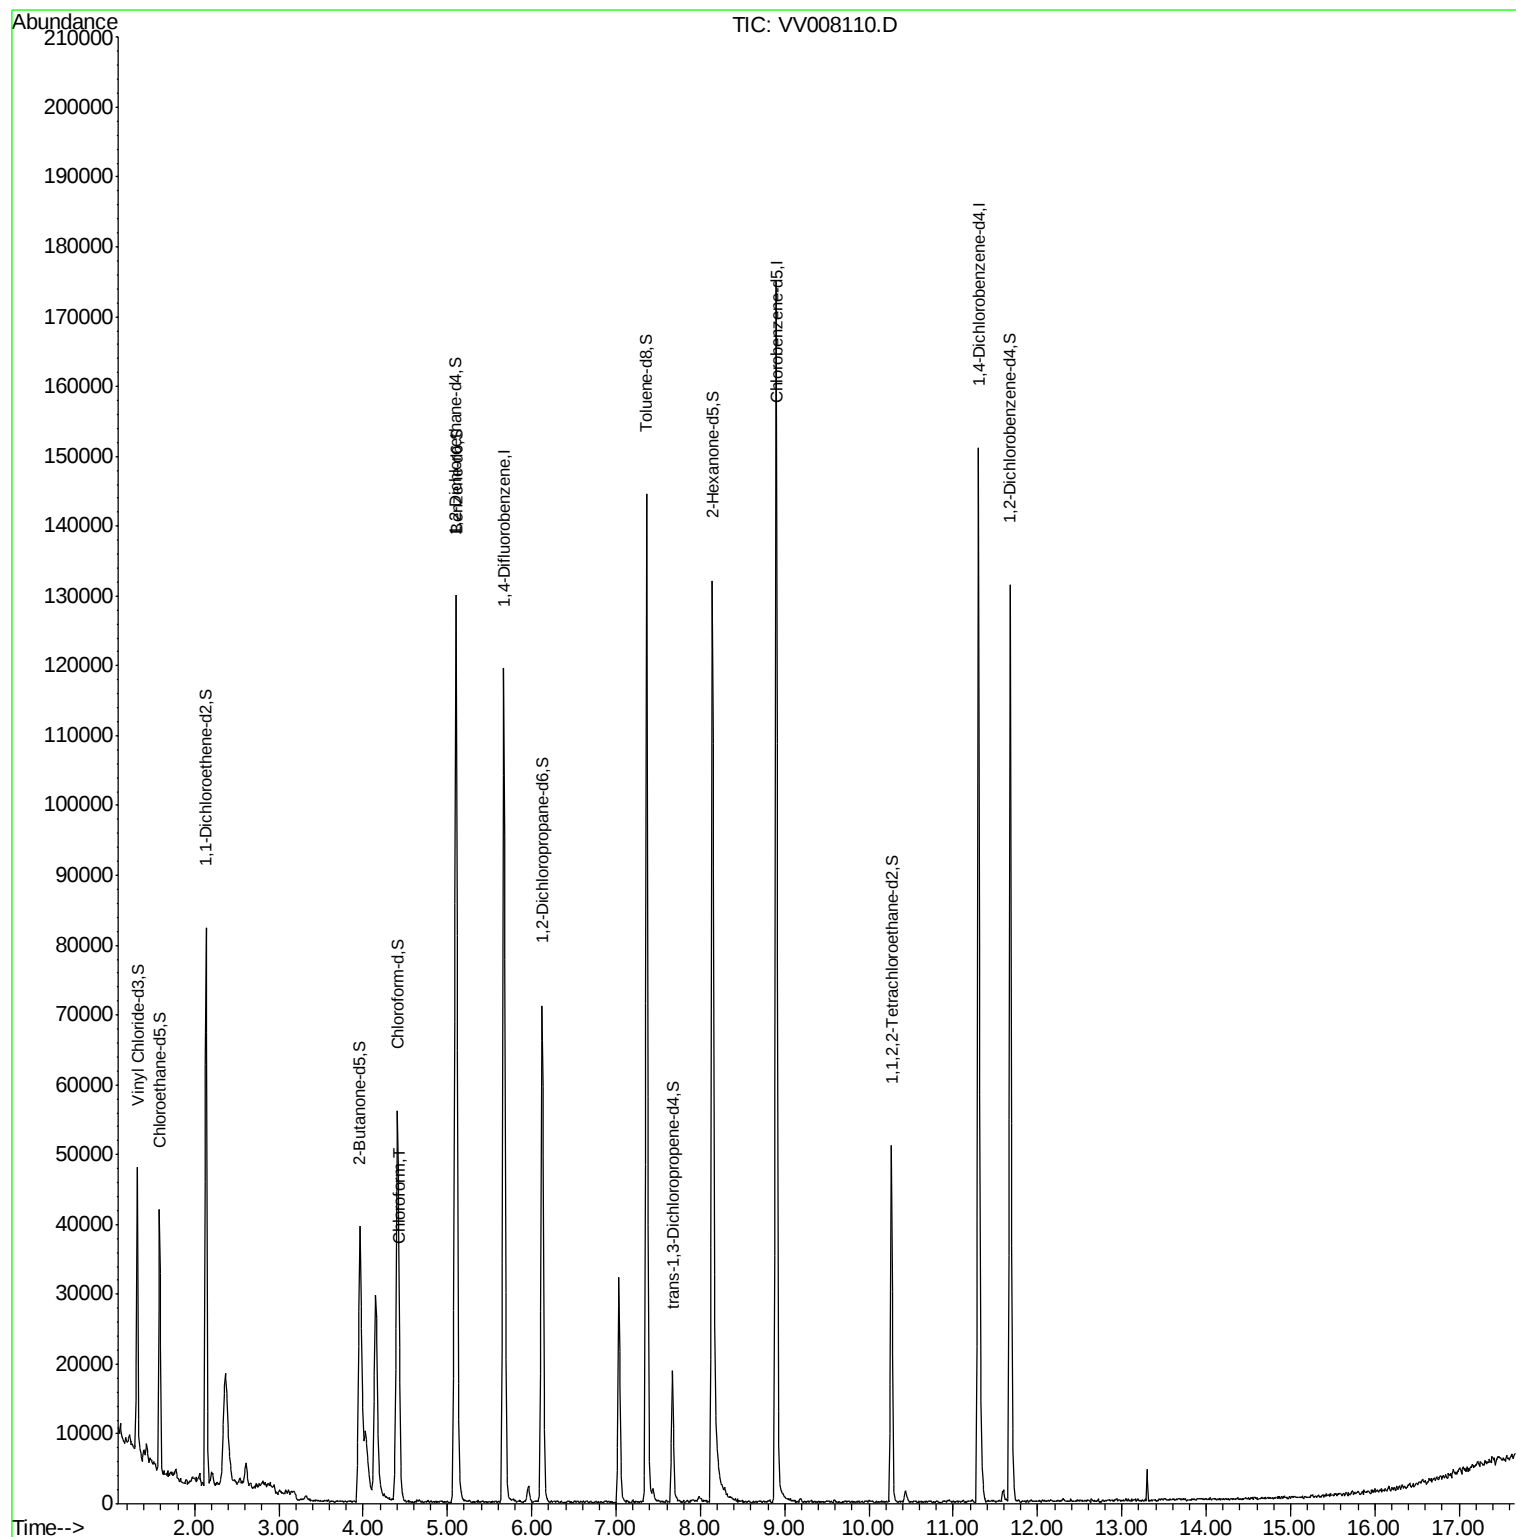

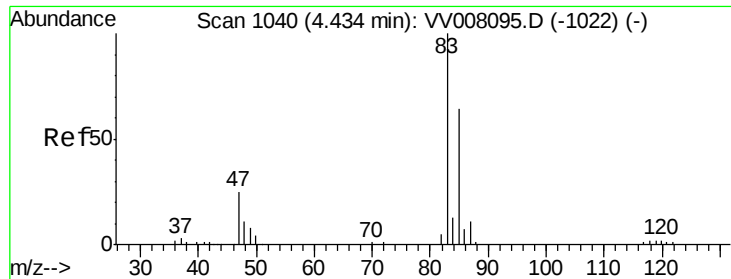

#25
 Chloroform
 Concen: 0.207 ug/L
 RT: 4.44 min Scan# 1041
 Delta R.T. 0.00 min
 Lab File: VV008110.D
 Acq: 05 Oct 2018 20:53

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYE2

Tot Ion: 83 Resp: 2576
 Ion Ratio Lower Upper
 83 100
 85 65.8 44.6 82.8

