

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008115.D
 Acq On : 05 Oct 2018 23:10
 Operator : SY/MD
 Sample : J5278-10
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYE7

Quant Time: Oct 06 03:22:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 01:03:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	103892	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	100656	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	45452	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27996	4.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.80%
7) Chloroethane-d5	1.59	69	24437	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.80%
11) 1,1-Dichloroethene-d2	2.14	63	42521	3.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.20%
20) 2-Butanone-d5	3.96	46	74170	48.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.68%
24) Chloroform-d	4.41	84	59828	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.09	65	30609	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
32) Benzene-d6	5.10	84	115338	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
36) 1,2-Dichloropropane-d6	6.12	67	35622	4.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.40%
41) Toluene-d8	7.36	98	104545	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.60%
43) trans-1,3-Dichloropropene-	7.67	79	11404	4.01	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.20%
46) 2-Hexanone-d5	8.14	63	51089	45.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.28%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	25482	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	42278	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	2626	2.526 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008115.D
Acq On : 05 Oct 2018 23:10
Operator : SY/MD
Sample : J5278-10
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE7

Quant Time: Oct 06 03:22:56 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 01:03:16 2018
Response via : Initial Calibration

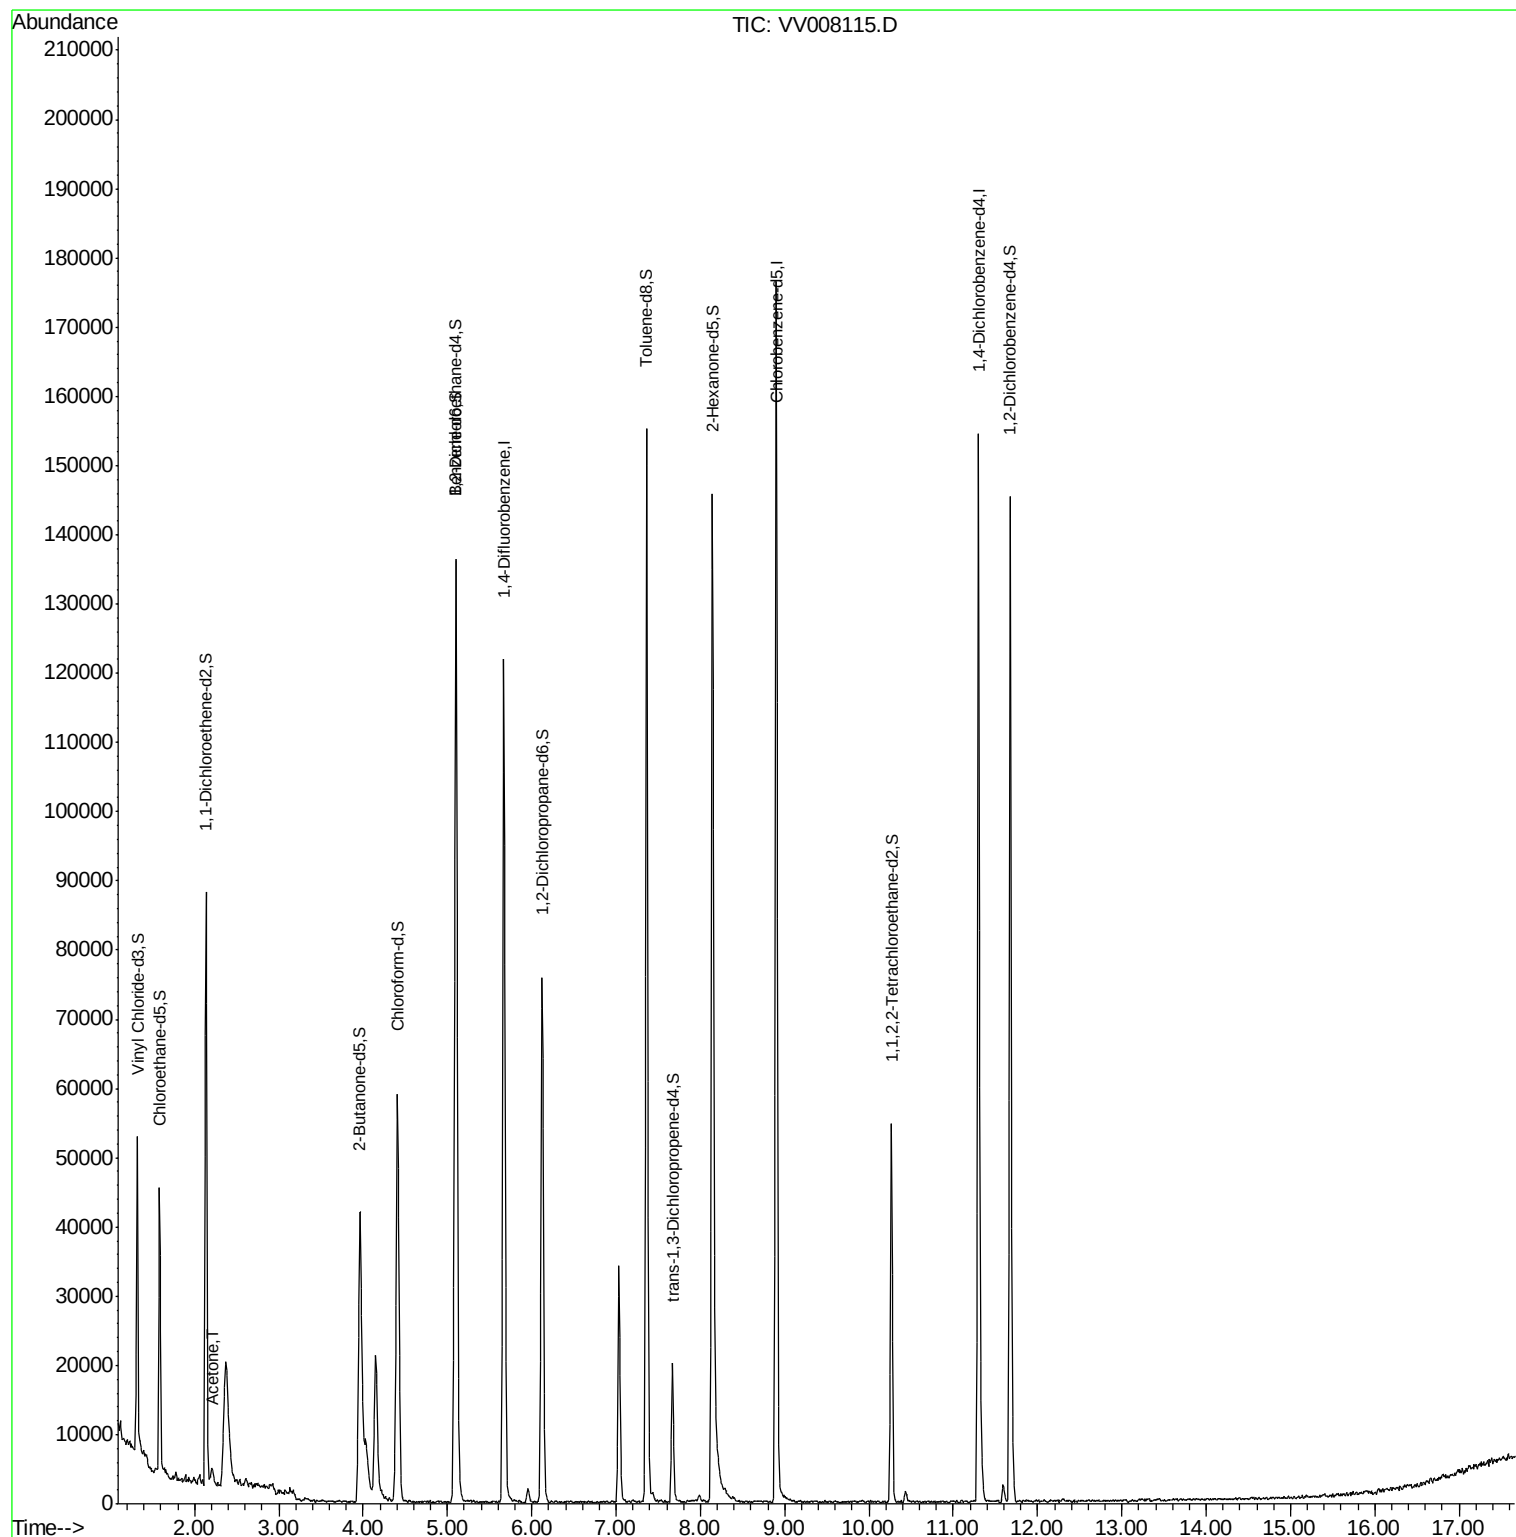

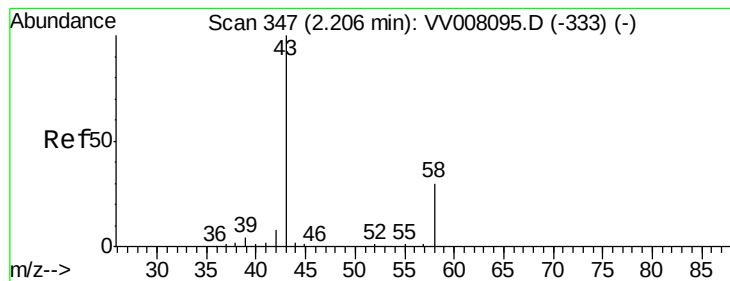

#13

Acetone

Concen: 2.526 ug/L

RT: 2.21 min Scan# 348

Delta R.T. 0.00 min

Lab File: VV008115.D

Acq: 05 Oct 2018 23:10

Instrument :
MSVOA_V
ClientSampleId :
BEYE7

Tot Ion: 43 Resp: 2626

Ion Ratio Lower Upper

43 100

58 25.3 0.0 62.2

