

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008124.D
 Acq On : 06 Oct 2018 03:16
 Operator : SY/MD
 Sample : J5277-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYB8

Quant Time: Oct 06 04:16:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 06 04:00:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	94321	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	85058	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	41445	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23722	4.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.00%
7) Chloroethane-d5	1.59	69	21473	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.00%
11) 1,1-Dichloroethene-d2	2.14	63	36737	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	3.96	46	68954	49.50	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.00%
24) Chloroform-d	4.41	84	53336	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.09	65	27256	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
32) Benzene-d6	5.10	84	100537	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.13	67	32965	4.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.60%
41) Toluene-d8	7.36	98	89593	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	7.67	79	9879	4.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.20%
46) 2-Hexanone-d5	8.14	63	45904	47.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.98%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22848	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	36935	4.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.00%


Target Compounds					Ovalue
13) Acetone	2.22	43	2536	2.687 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008124.D
Acq On : 06 Oct 2018 03:16
Operator : SY/MD
Sample : J5277-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYB8

Quant Time: Oct 06 04:16:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 06 04:00:29 2018
Response via : Initial Calibration

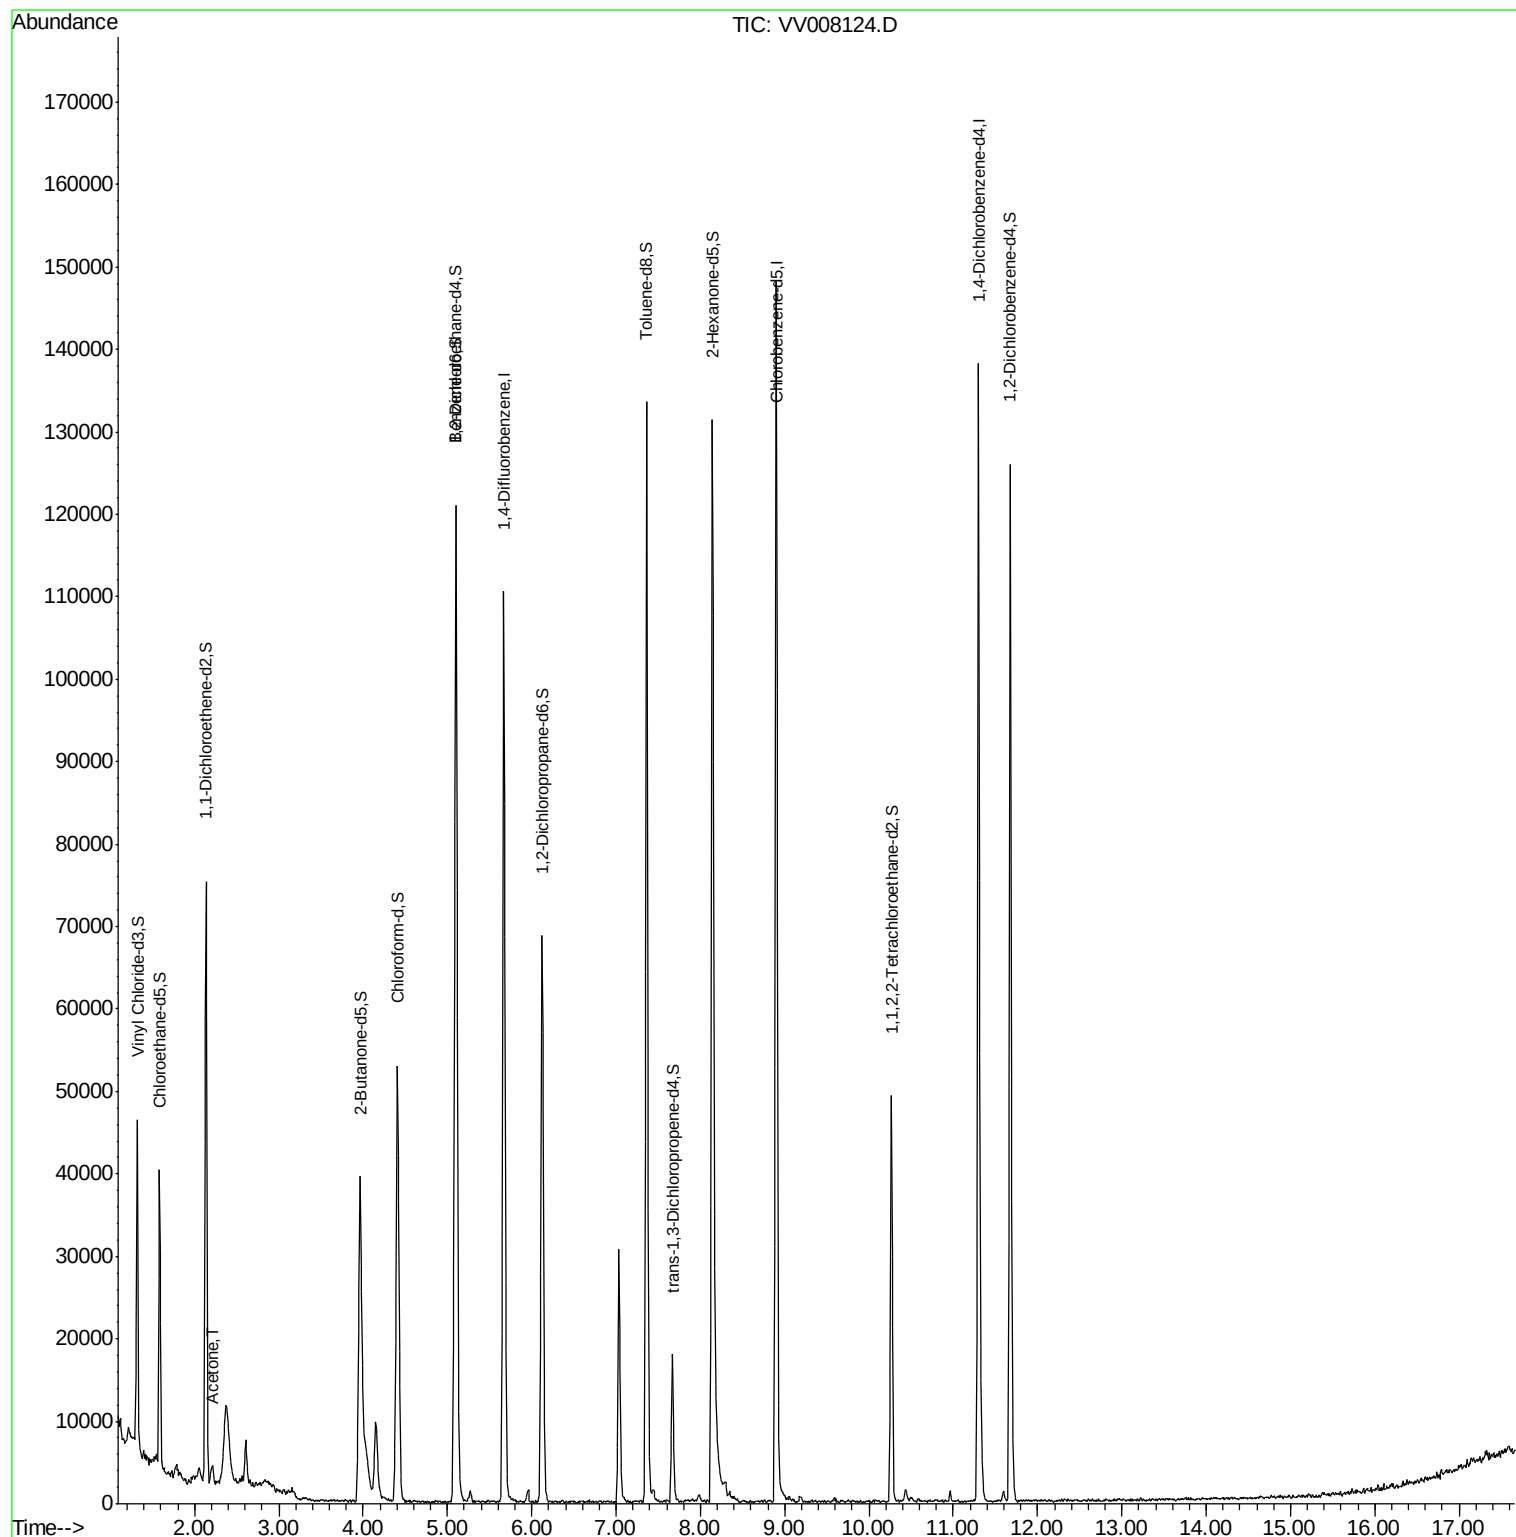

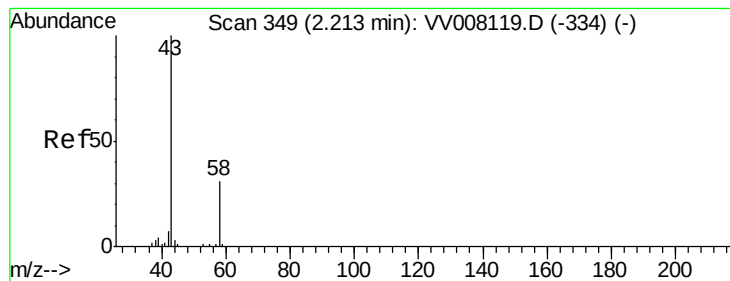

#13
 Acetone
 Concen: 2.687 ug/L
 RT: 2.22 min Scan# 350
 Delta R.T. 0.00 min
 Lab File: VV008124.D
 Acq: 06 Oct 2018 03:16

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYB8

Tot Ion: 43 Resp: 2536
 Ion Ratio Lower Upper
 43 100
 58 24.5 0.0 62.2

