

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008135.D
 Acq On : 06 Oct 2018 08:16
 Operator : SY/MD
 Sample : J5277-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYC9

Quant Time: Oct 08 05:50:23 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 08 05:22:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	93673	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	90926	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40447	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23571	4.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.00%
7) Chloroethane-d5	1.59	69	21969	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.60%
11) 1,1-Dichloroethene-d2	2.14	63	35665	3.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.40%
20) 2-Butanone-d5	3.96	46	70441	50.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.84%
24) Chloroform-d	4.41	84	53567	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
26) 1,2-Dichloroethane-d4	5.09	65	27926	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
32) Benzene-d6	5.10	84	100842	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
36) 1,2-Dichloropropane-d6	6.12	67	32850	4.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.20%
41) Toluene-d8	7.36	98	87707	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
43) trans-1,3-Dichloropropene-	7.67	79	9727	3.79	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.80%
46) 2-Hexanone-d5	8.14	63	46606	45.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.16%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	22944	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	36989	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	2258	2.409 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008135.D
Acq On : 06 Oct 2018 08:16
Operator : SY/MD
Sample : J5277-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYC9

Quant Time: Oct 08 05:50:23 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 08 05:22:34 2018
Response via : Initial Calibration

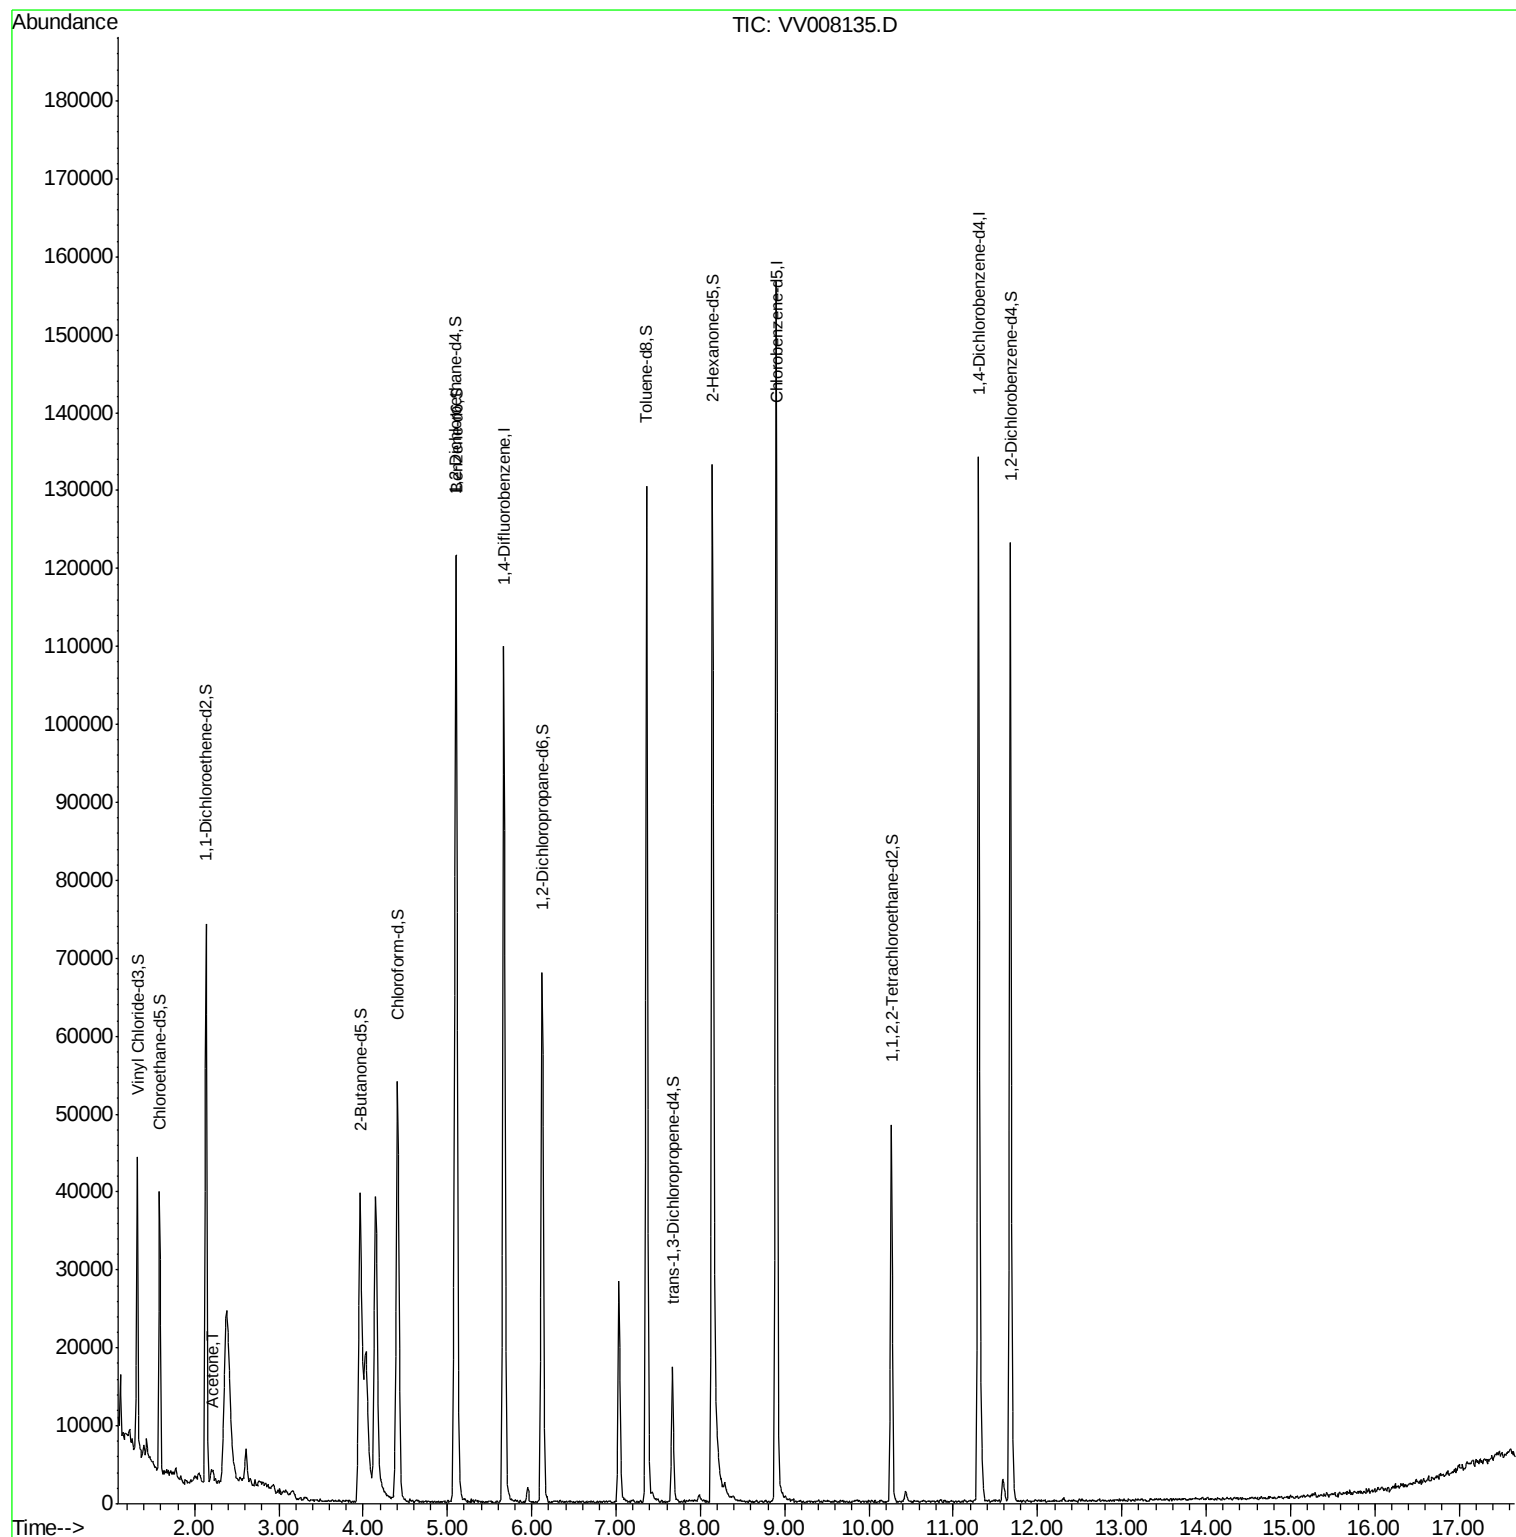

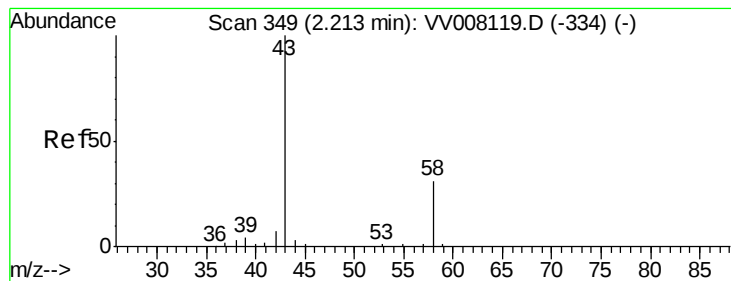

#13
 Acetone
 Concen: 2.409 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. -0.00 min
 Lab File: VV008135.D
 Acq: 06 Oct 2018 08:16

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYC9

Tot Ion: 43 Resp: 2258
 Ion Ratio Lower Upper
 43 100
 58 27.2 0.0 62.2

