

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008136.D
 Acq On : 06 Oct 2018 08:44
 Operator : SY/MD
 Sample : J5277-13
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYD0

Quant Time: Oct 08 05:53:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 08 05:22:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	95471	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	92485	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	41272	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24460	4.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.40%
7) Chloroethane-d5	1.59	69	21950	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.80%
11) 1,1-Dichloroethene-d2	2.14	63	36872	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.96	46	73847	52.38	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.76%
24) Chloroform-d	4.41	84	55909	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.09	65	28809	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
32) Benzene-d6	5.10	84	104903	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
36) 1,2-Dichloropropane-d6	6.12	67	34141	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.36	98	91072	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.20%
43) trans-1,3-Dichloropropene-	7.67	79	10533	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	8.14	63	47853	46.01	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.02%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	24120	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	38161	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	2251	2.356 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008136.D
Acq On : 06 Oct 2018 08:44
Operator : SY/MD
Sample : J5277-13
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYD0

Quant Time: Oct 08 05:53:26 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 08 05:22:34 2018
Response via : Initial Calibration

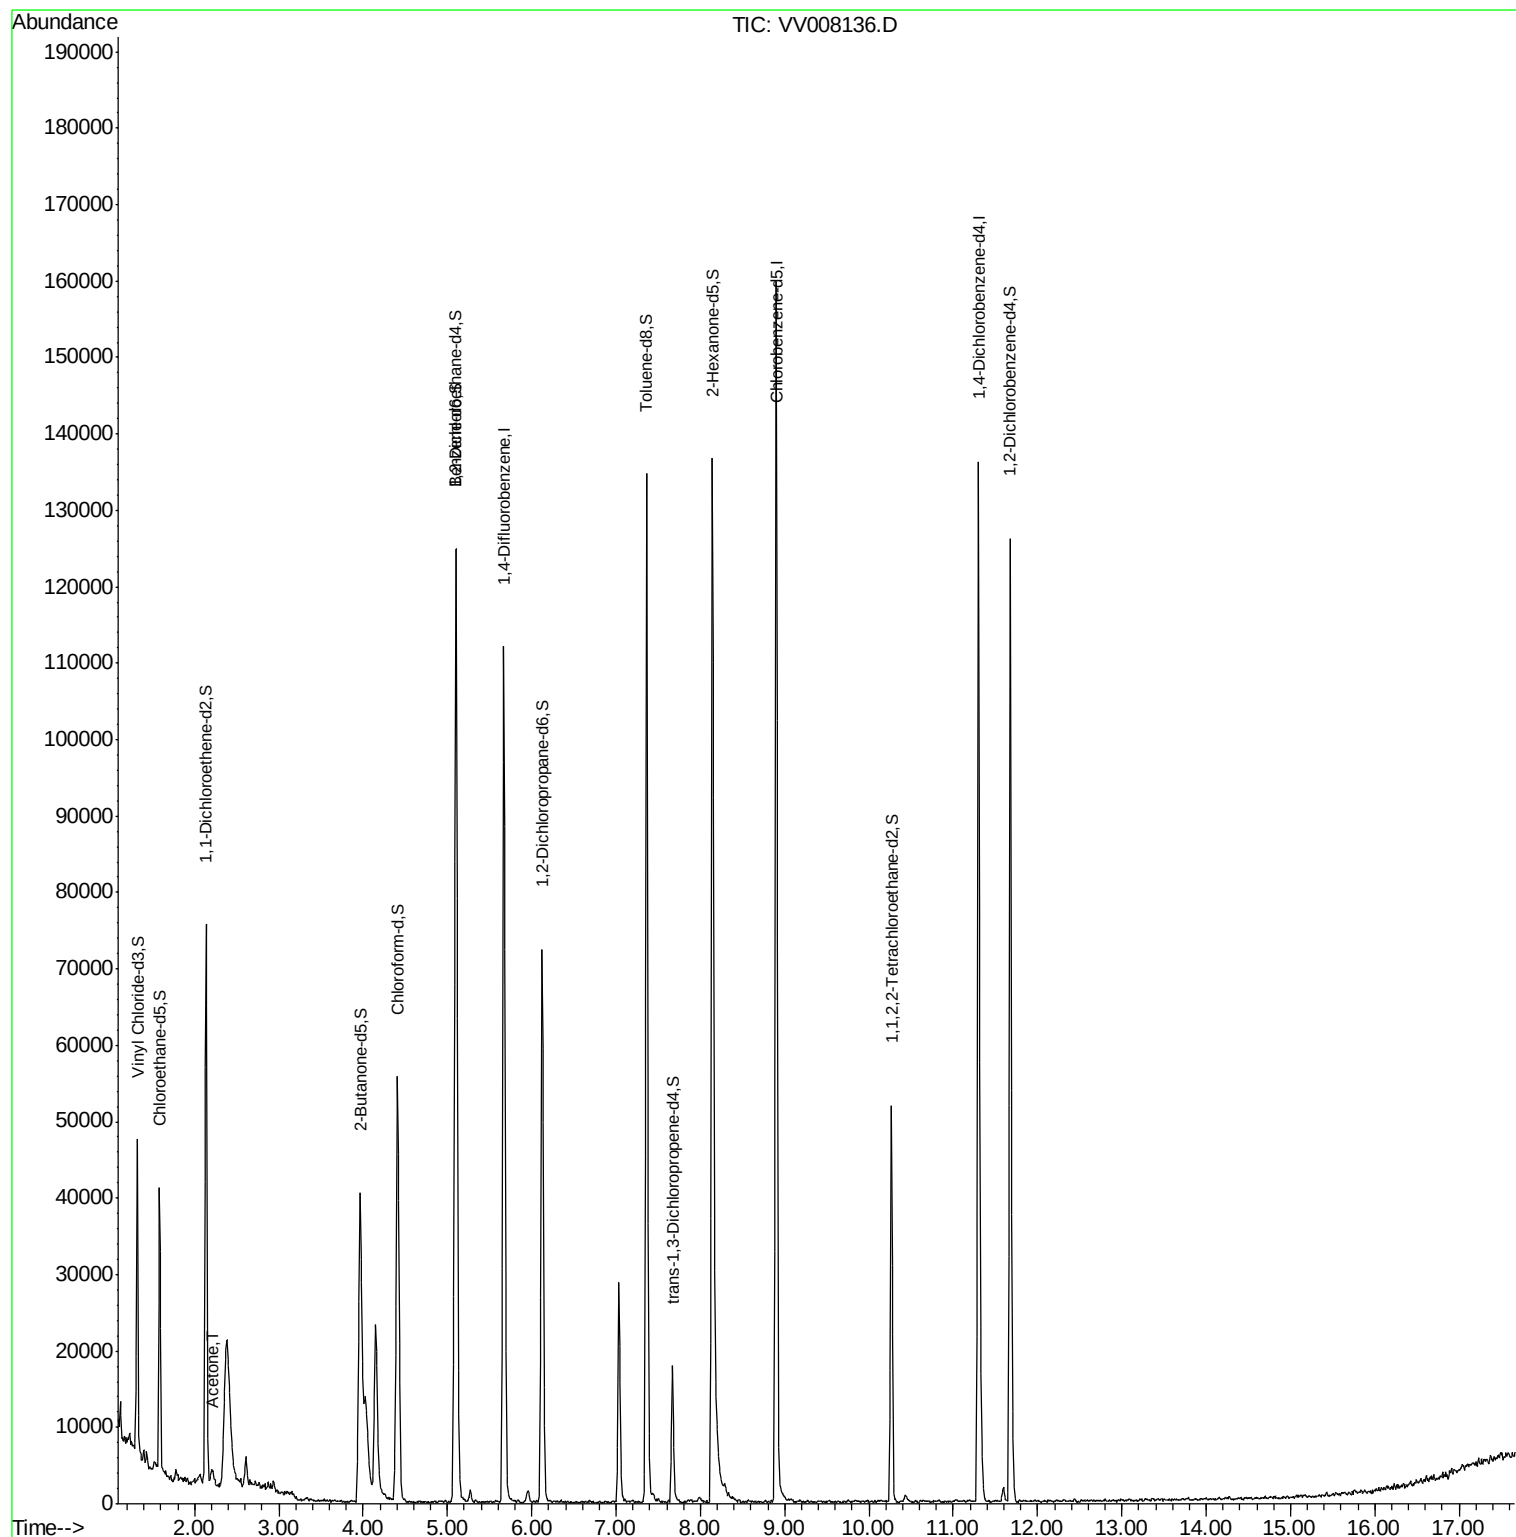

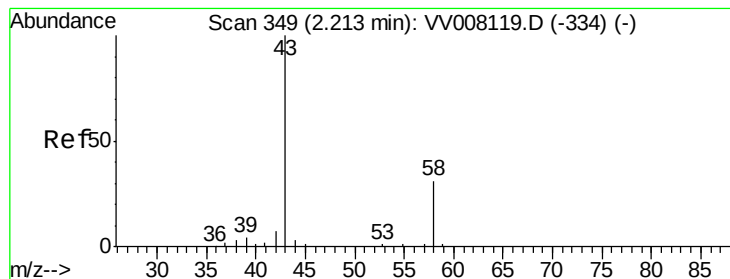

#13
 Acetone
 Concen: 2.356 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. -0.00 min
 Lab File: VV008136.D
 Acq: 06 Oct 2018 08:44

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYD0

Tot Ion: 43 Resp: 2251
 Ion Ratio Lower Upper
 43 100
 58 28.8 0.0 62.2

