

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008098.D
 Acq On : 05 Oct 2018 15:15
 Operator : SY/MD
 Sample : J5246-11RE
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J79RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	63	72	90	rVB	44399	53219	17.23%	1.787%
2	1.431	100	106	116	rVB	19721	22180	7.18%	0.745%
3	1.585	147	154	165	rVB	39452	45360	14.69%	1.524%
4	2.135	314	325	336	rBV	83086	120836	39.13%	4.059%
5	2.364	380	396	422	rVB2	9075	32961	10.67%	1.107%
6	3.962	878	893	904	rBV	42938	115007	37.24%	3.863%
7	4.409	1016	1032	1057	rVB	56678	137041	44.38%	4.603%
8	4.878	1165	1178	1194	rBV5	3635	8730	2.83%	0.293%
9	5.100	1229	1247	1272	rBV2	127293	300156	97.20%	10.081%
10	5.669	1410	1424	1442	rBV	130849	253483	82.08%	8.514%
11	5.965	1504	1516	1534	rVB2	32665	63402	20.53%	2.129%
12	6.122	1552	1565	1594	rBV	71694	143140	46.35%	4.808%
13	7.035	1834	1849	1868	rBV	35009	62385	20.20%	2.095%
14	7.363	1936	1951	1968	rBV	147896	258612	83.74%	8.686%
15	7.434	1968	1973	1985	rVB4	2692	4824	1.56%	0.162%
16	7.669	2035	2046	2060	rBV	19763	34637	11.22%	1.163%
17	7.987	2132	2145	2147	rBV2	10156	13725	4.44%	0.461%
18	8.023	2149	2156	2168	rVB2	27643	46172	14.95%	1.551%
19	8.142	2181	2193	2226	rBV	138841	282036	91.33%	9.473%
20	8.900	2417	2429	2454	rBV	184653	308815	100.00%	10.372%
21	10.267	2842	2854	2866	rBV2	52250	81025	26.24%	2.721%
22	10.431	2893	2905	2921	rBV	29334	50541	16.37%	1.698%
23	11.299	3164	3175	3207	rVB	172077	291880	94.52%	9.803%
24	11.675	3281	3292	3313	rBV	139805	232021	75.13%	7.793%
25	12.305	3477	3488	3497	rBV3	5176	8345	2.70%	0.280%
26	16.765	4869	4875	4882	rBV5	5228	6804	2.20%	0.229%


Sum of corrected areas: 2977337

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008098.D
Acq On : 05 Oct 2018 15:15
Operator : SY/MD
Sample : J5246-11RE
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J79RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

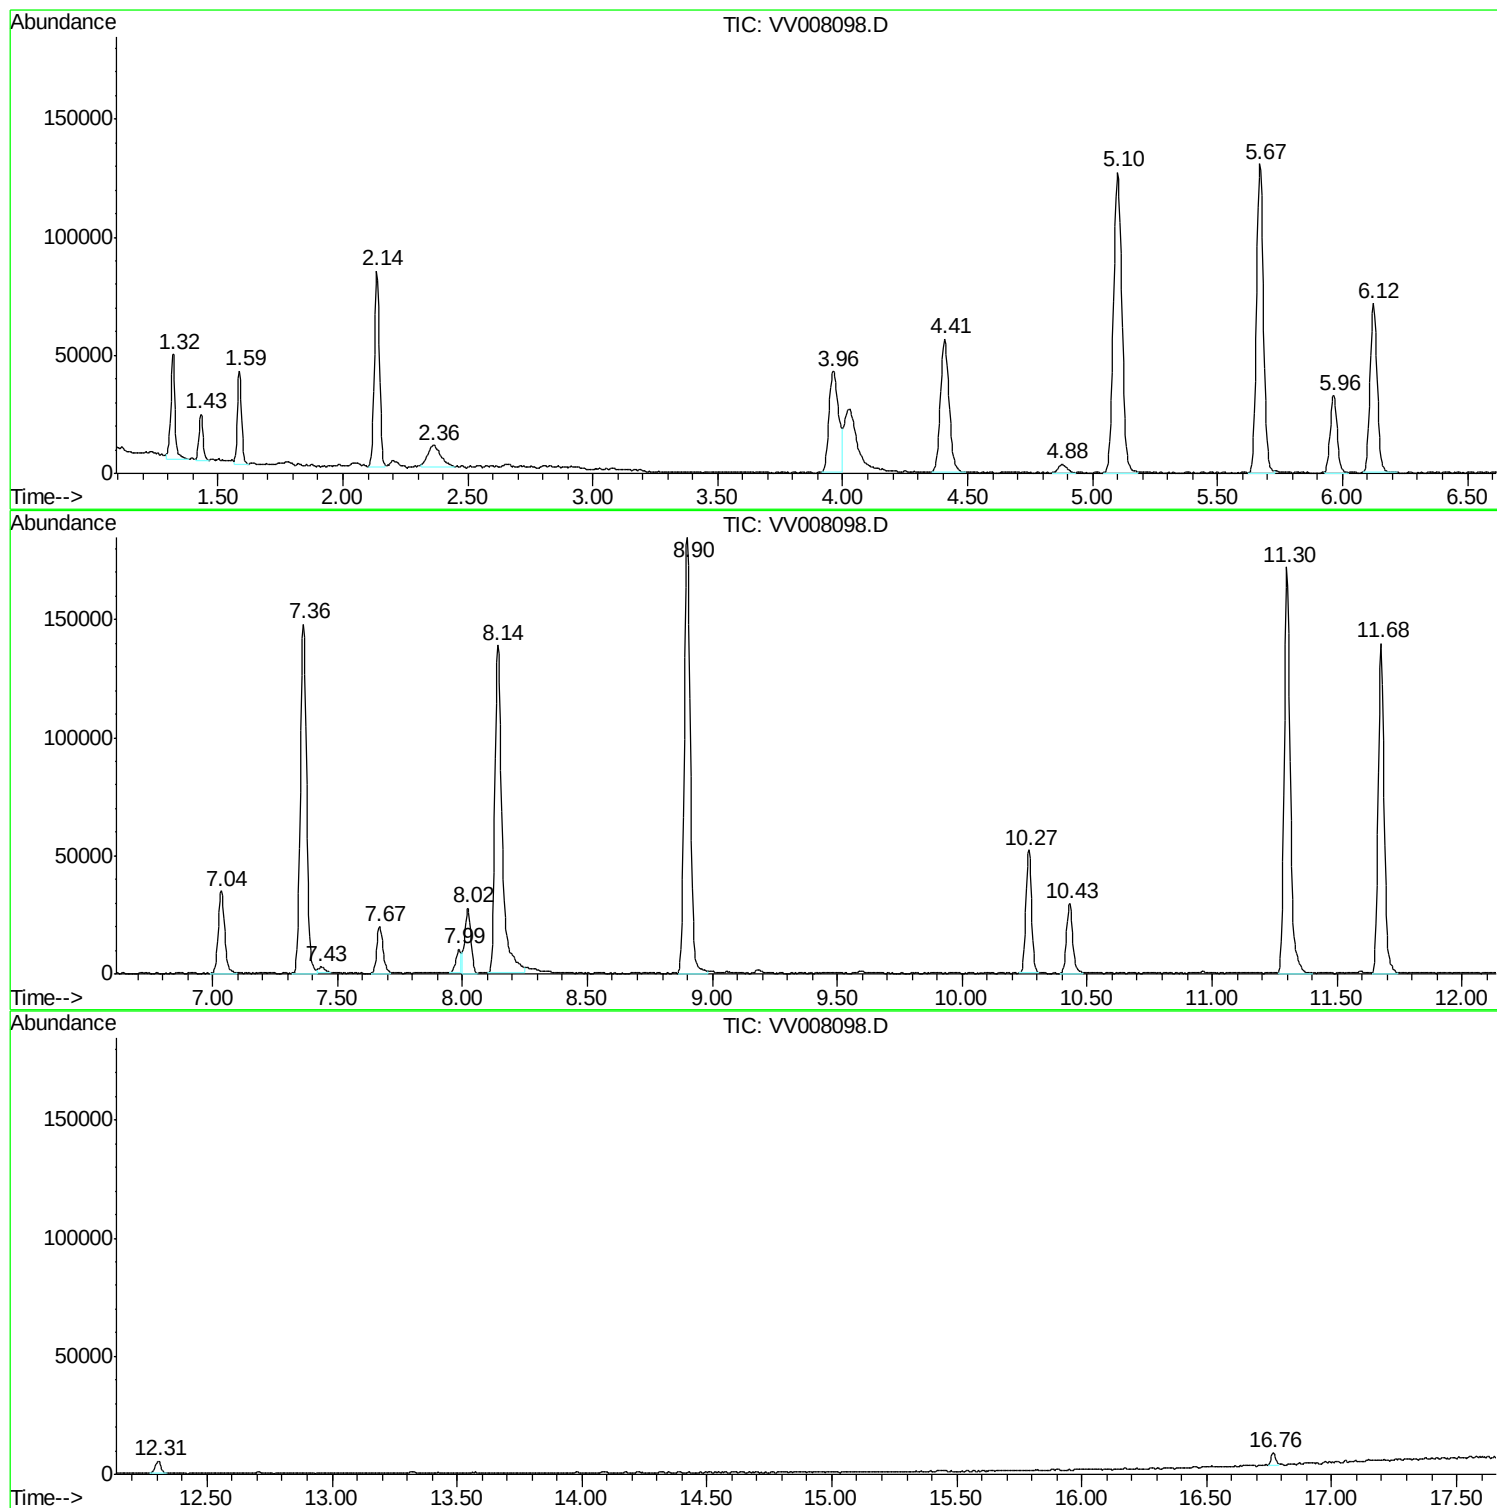

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008098.D
Acq On : 05 Oct 2018 15:15
Operator : SY/MD
Sample : J5246-11RE
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J79RE










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.36	0.65 ug/L	32961	1,4-Difluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
3			4-Penten-2-ol	86	C5H10O	000625-31-0	9
4			Methane, nitroso-	45	CH3NO	000865-40-7	4
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

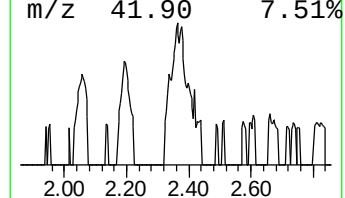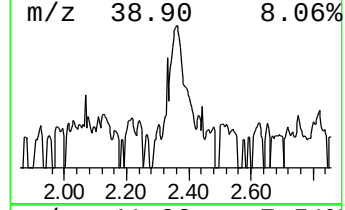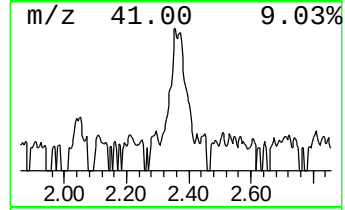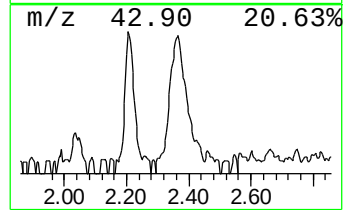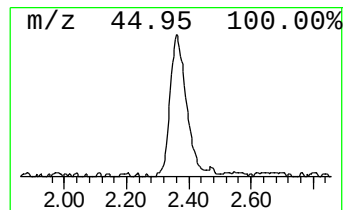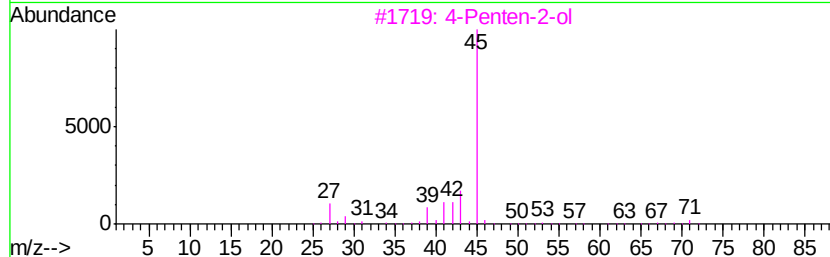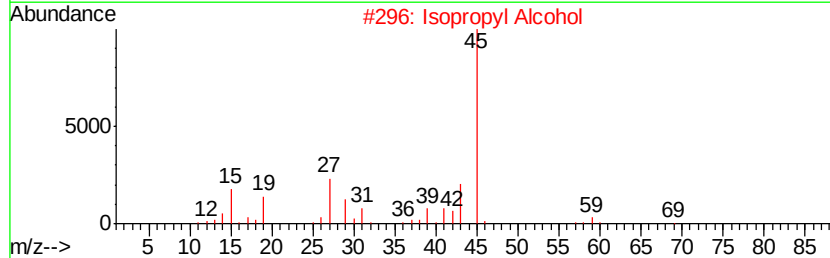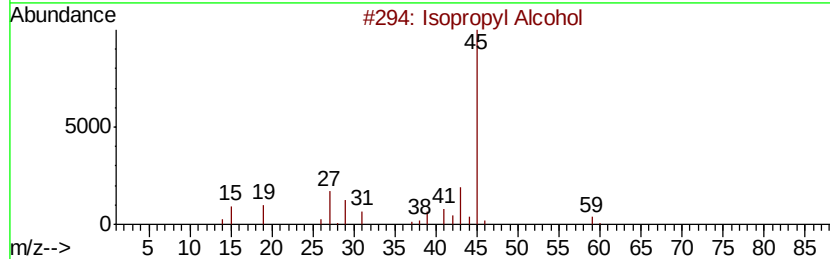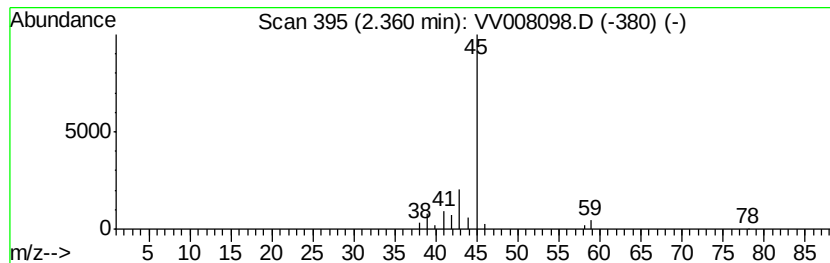

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100518\
Data File : VV008098.D
Acq On : 05 Oct 2018 15:15
Operator : SY/MD
Sample : J5246-11RE
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J79RE

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.36	0.7	ug/L	32961	1	5.67	253483	5.0