

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008108.D
 Acq On : 05 Oct 2018 19:58
 Operator : SY/MD
 Sample : J5278-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	83	rVB	44113	51230	16.55%	1.867%
2	1.431	102	106	114	rVB2	3728	4196	1.36%	0.153%
3	1.586	147	154	167	rVB	39178	44278	14.31%	1.613%
4	2.135	314	325	337	rBV	81668	115642	37.36%	4.214%
5	2.200	341	345	355	rVB6	1960	3229	1.04%	0.118%
6	2.373	376	399	428	rBV2	20158	87070	28.13%	3.173%
7	3.962	878	893	907	rBV	40545	109627	35.42%	3.994%
8	4.155	942	953	970	rVB2	4021	9699	3.13%	0.353%
9	4.409	1015	1032	1053	rBV	56988	134926	43.59%	4.916%
10	5.100	1228	1247	1267	rBV2	132977	309509	100.00%	11.277%
11	5.669	1409	1424	1444	rBV	120347	234034	75.61%	8.527%
12	5.955	1503	1513	1524	rVB7	1813	3278	1.06%	0.119%
13	6.122	1552	1565	1587	rBV	72811	145916	47.14%	5.317%
14	7.036	1838	1849	1865	rBV	34759	60417	19.52%	2.201%
15	7.364	1936	1951	1967	rBV	148196	254600	82.26%	9.277%
16	7.669	2036	2046	2059	rBV	19501	32780	10.59%	1.194%
17	8.142	2180	2193	2226	rBV2	137187	285509	92.25%	10.403%
18	8.900	2416	2429	2465	rBV	173192	285824	92.35%	10.414%
19	10.267	2842	2854	2874	rBV	51222	82267	26.58%	2.998%
20	11.299	3164	3175	3200	rBV	149004	255977	82.70%	9.327%
21	11.592	3258	3266	3277	rVB6	2877	5393	1.74%	0.197%
22	11.675	3281	3292	3313	rBV	138389	229119	74.03%	8.348%


Sum of corrected areas: 2744520

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008108.D
Acq On : 05 Oct 2018 19:58
Operator : SY/MD
Sample : J5278-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

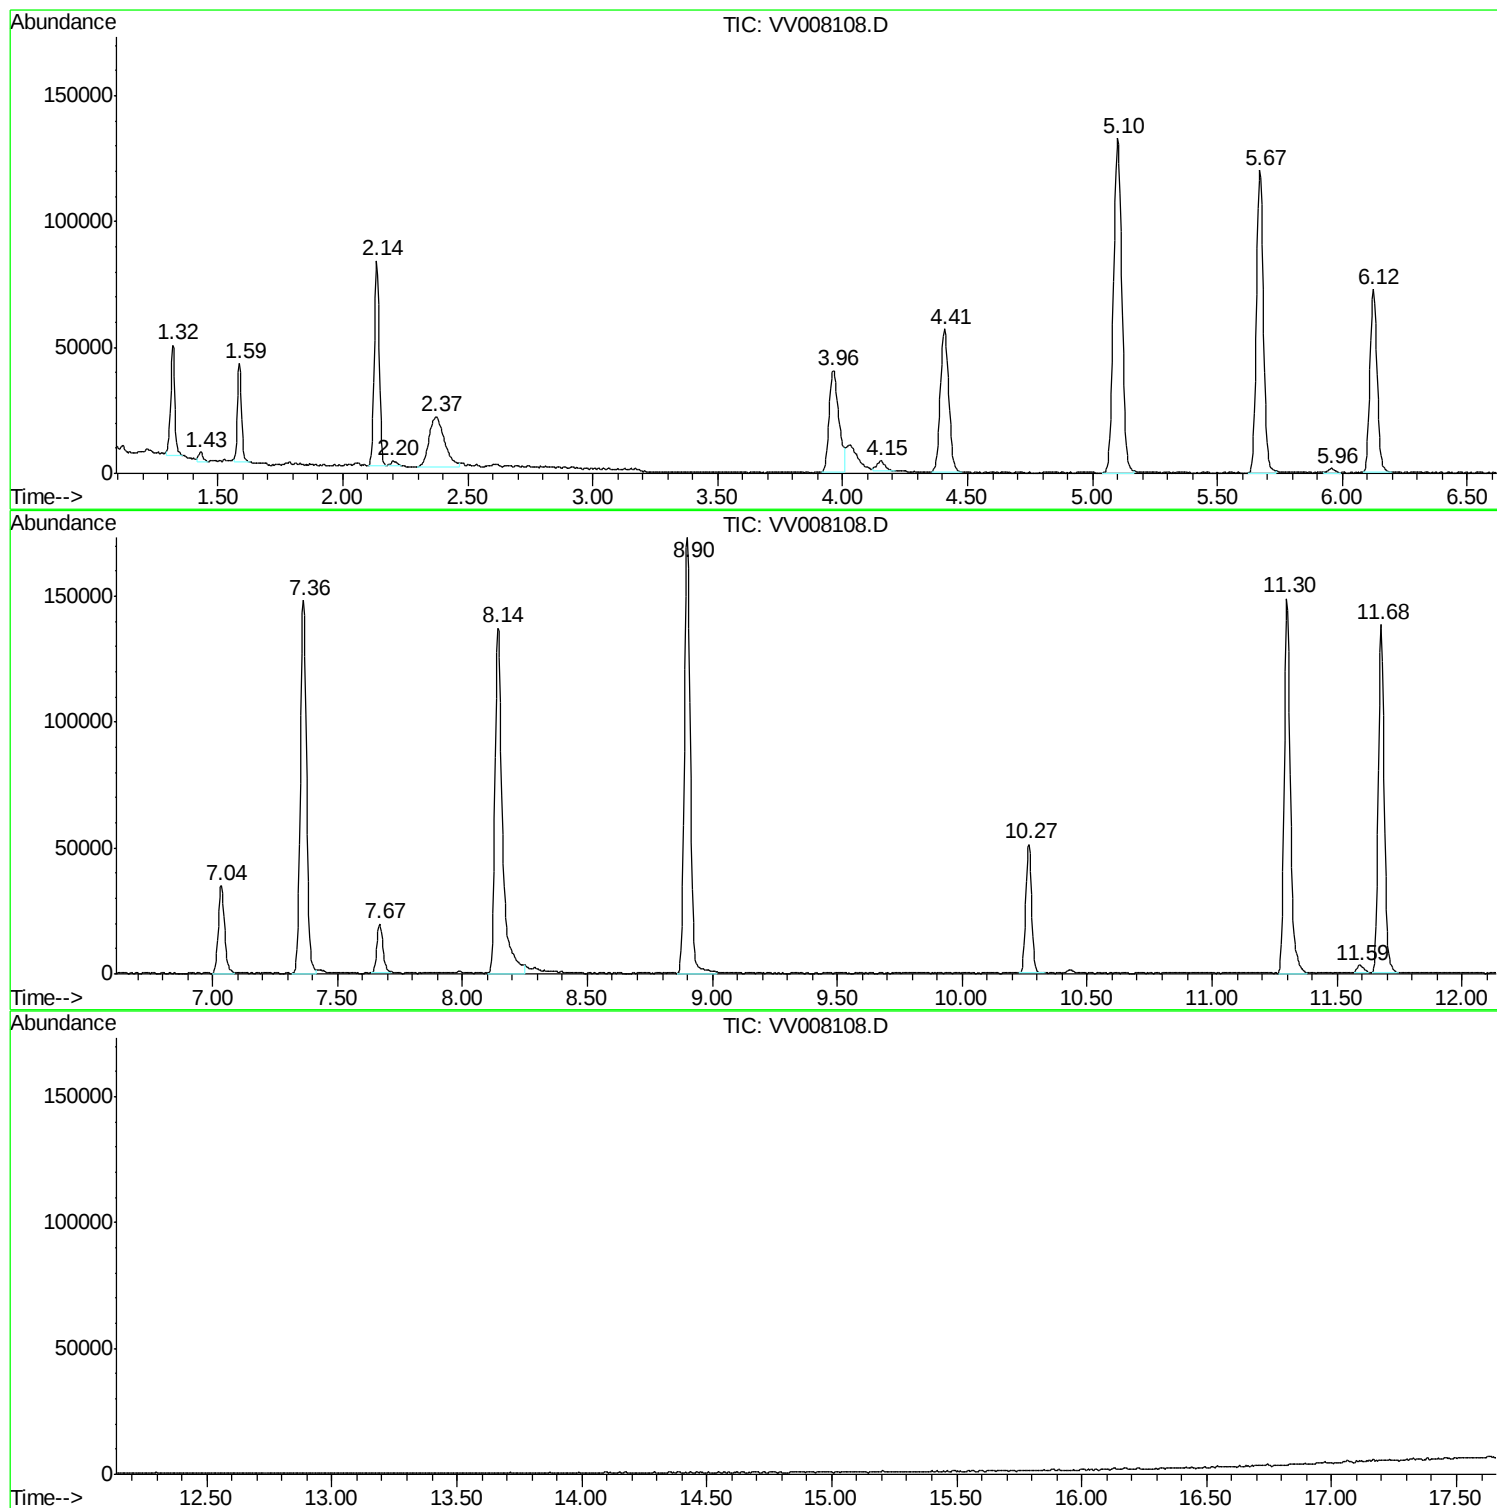

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008108.D
Acq On : 05 Oct 2018 19:58
Operator : SY/MD
Sample : J5278-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE0










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.37	1.86 ug/L	87070	1,4-Difluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	74
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	9
4		2,3-Butanediol	90	C4H10O2	000513-85-9	4
5		Isopropyl Alcohol	60	C3H8O	000067-63-0	4

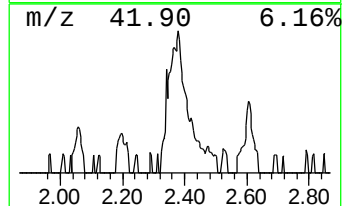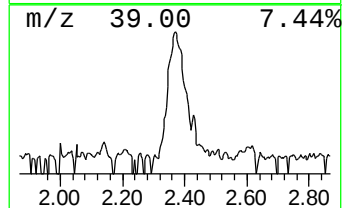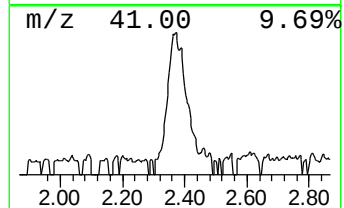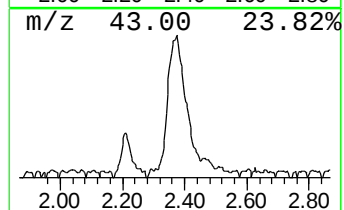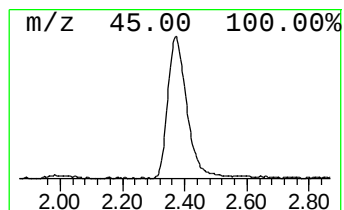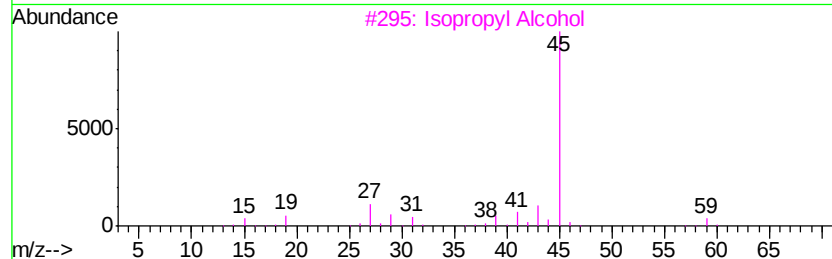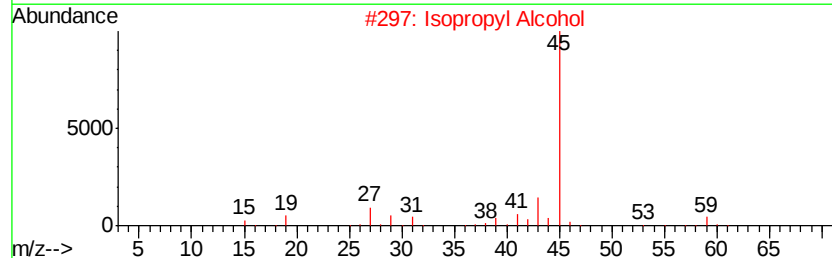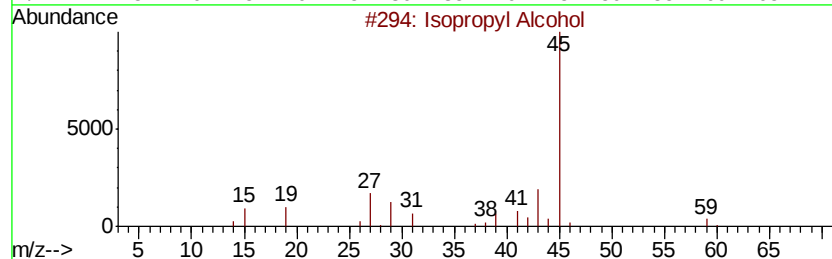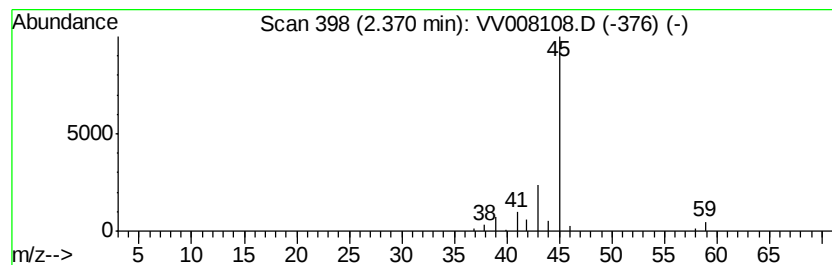

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100518\
Data File : VV008108.D
Acq On : 05 Oct 2018 19:58
Operator : SY/MD
Sample : J5278-03
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.37	1.9	ug/L	87070	1	5.67	234034	5.0