

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
 Data File : VV008111.D
 Acq On : 05 Oct 2018 21:20
 Operator : SY/MD
 Sample : J5278-06
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEYE3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	83	rVB	43717	49442	15.71%	1.769%
2	1.586	147	154	164	rVB	40028	45481	14.45%	1.628%
3	2.135	315	325	338	rVB	83799	117589	37.36%	4.208%
4	2.203	338	346	354	rBV4	2055	3690	1.17%	0.132%
5	2.364	379	396	426	rBV	21981	80813	25.67%	2.892%
6	3.962	878	893	907	rBV2	40927	112424	35.71%	4.023%
7	4.151	941	952	970	rVB3	6303	16089	5.11%	0.576%
8	4.409	1016	1032	1050	rBV	58980	135981	43.20%	4.866%
9	5.100	1228	1247	1269	rBV2	134878	314782	100.00%	11.265%
10	5.669	1410	1424	1444	rBV	124367	239361	76.04%	8.566%
11	5.958	1504	1514	1523	rVB7	1872	3400	1.08%	0.122%
12	6.122	1552	1565	1584	rBV	74912	147697	46.92%	5.285%
13	7.035	1836	1849	1868	rBV	34615	60643	19.27%	2.170%
14	7.363	1937	1951	1970	rBV	152061	262830	83.50%	9.406%
15	7.669	2030	2046	2067	rBV	20124	34985	11.11%	1.252%
16	8.142	2181	2193	2230	rBV2	141197	293250	93.16%	10.494%
17	8.900	2413	2429	2452	rBV	175955	293360	93.19%	10.498%
18	10.267	2842	2854	2868	rBV	53661	84135	26.73%	3.011%
19	10.431	2895	2905	2921	rBV5	2013	4305	1.37%	0.154%
20	11.299	3161	3175	3200	rBV	153690	261654	83.12%	9.363%
21	11.675	3280	3292	3316	rVB	138840	232499	73.86%	8.320%


Sum of corrected areas: 2794410

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008111.D
Acq On : 05 Oct 2018 21:20
Operator : SY/MD
Sample : J5278-06
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

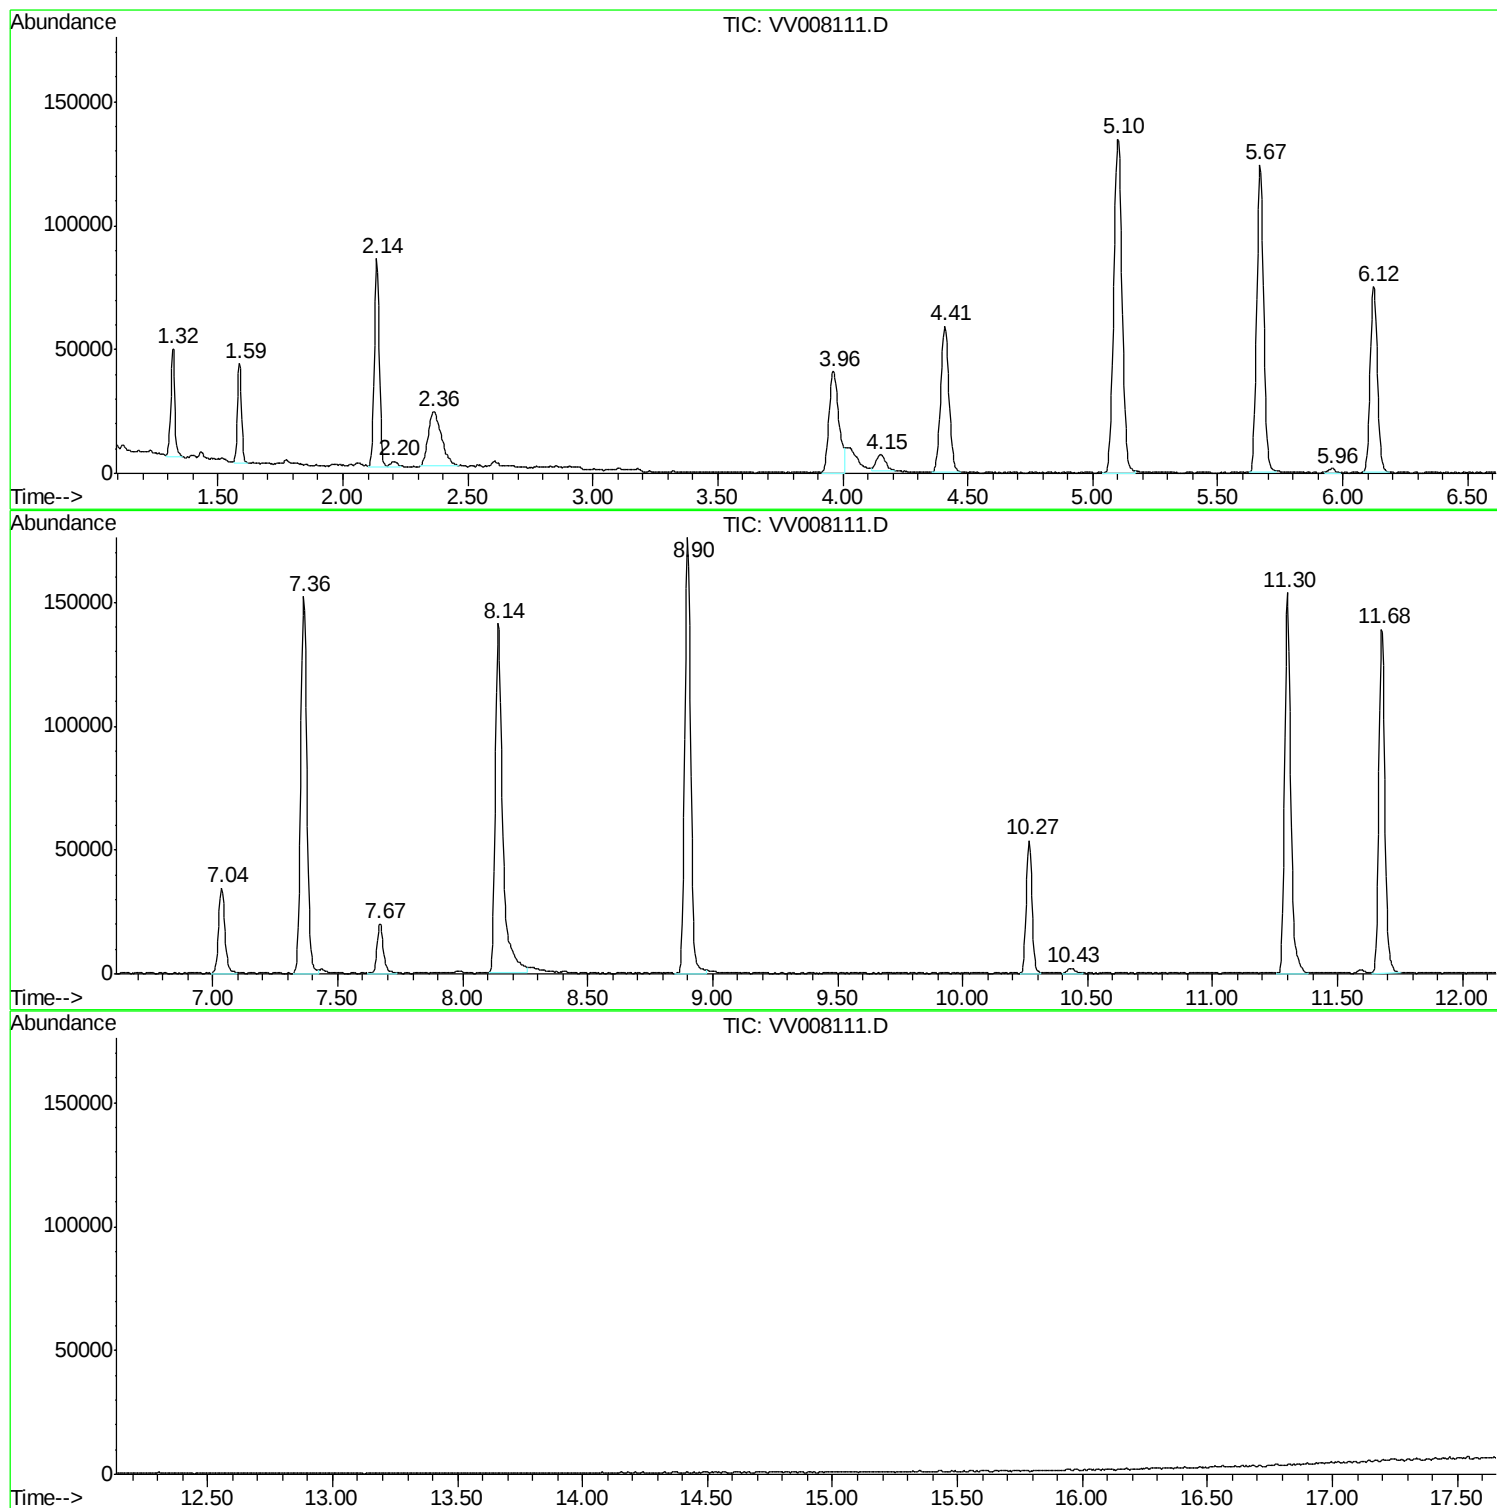

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008111.D
Acq On : 05 Oct 2018 21:20
Operator : SY/MD
Sample : J5278-06
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE3










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-ethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.36	1.69 ug/L	80813	1,4-Difluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	74
2			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	64
3			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	43
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	43
5			(S)-(+)-2-Pentanol	88	C5H12O	026184-62-3	9

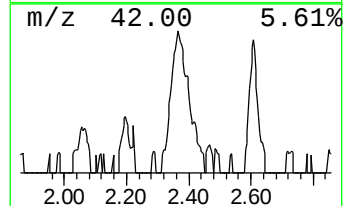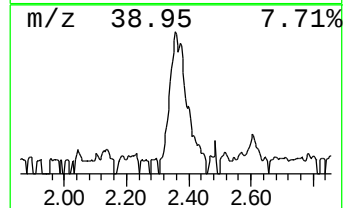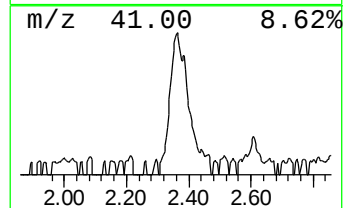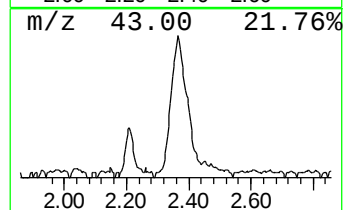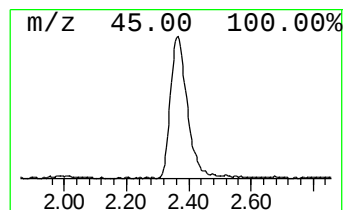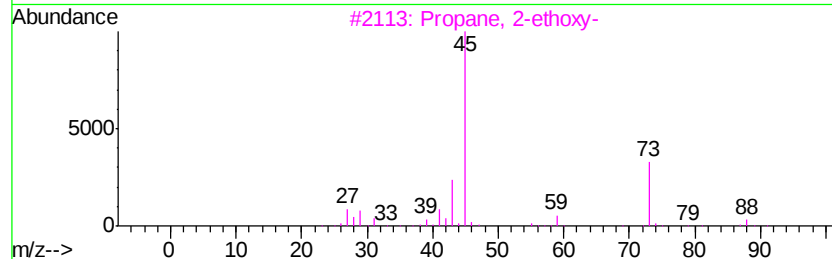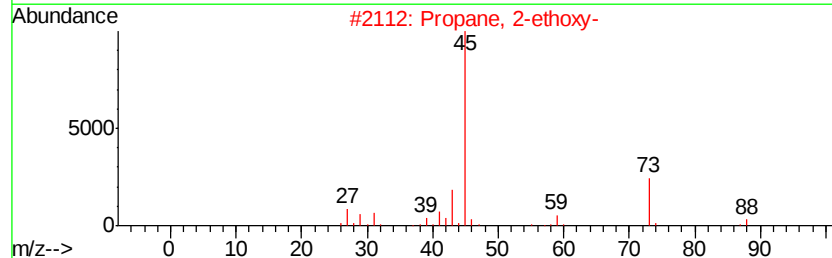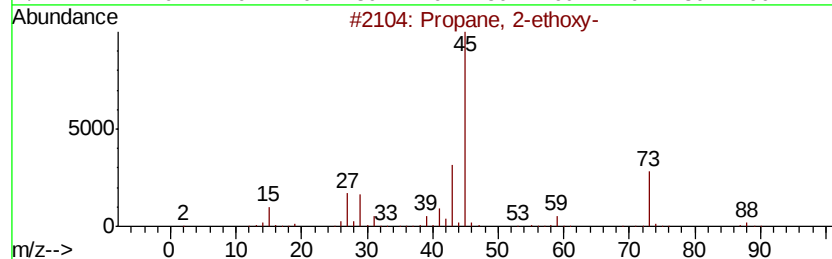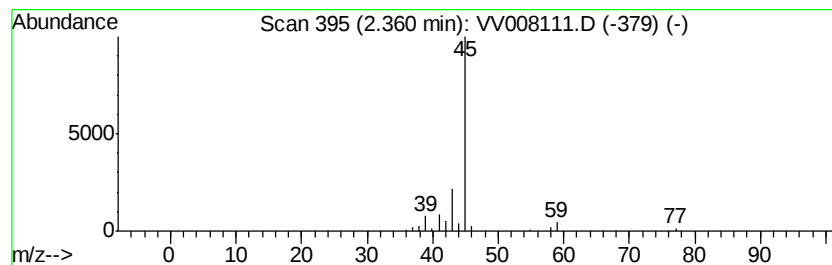

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV100518\
Data File : VV008111.D
Acq On : 05 Oct 2018 21:20
Operator : SY/MD
Sample : J5278-06
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEYE3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-ethoxy-	2.36	1.7	ug/L	80813	1	5.67	239361	5.0