


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100518\
Data File : VV008087.D
Acq On : 05 Oct 2018 09:07
Operator : SY/MD
Sample : BFB82
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB82

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR100518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 09 04:07:48 2018

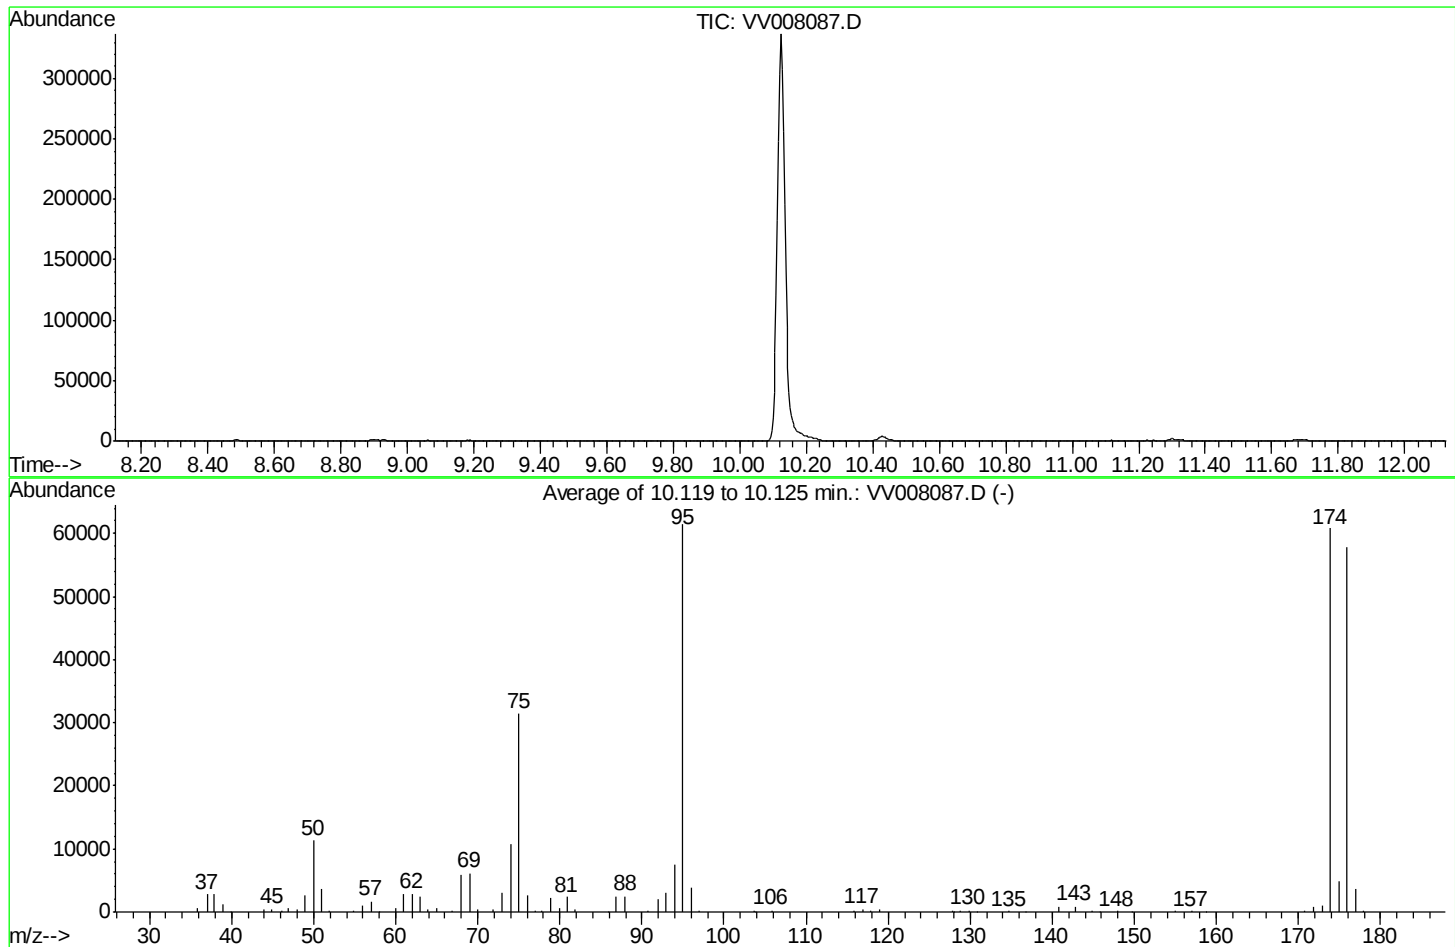

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	11274	PASS
75	95	30	80	51.1	31378	PASS
95	95	100	100	100.0	61458	PASS
96	95	5	9	6.2	3826	PASS
173	174	0.00	2	1.6	946	PASS
174	95	50	120	98.9	60797	PASS
175	174	5	9	7.9	4818	PASS
176	174	95	101	95.2	57906	PASS
177	176	5	9	6.4	3707	PASS

Scan 2796 (10.080 min): VV008087.D
BFB82

m/z	Abundance
39.90	142.0
43.90	290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	473.0
37.00	2667.0
37.90	2655.0
38.90	1106.0
39.90	171.0
43.90	586.0
44.90	469.0
46.00	140.0
46.90	629.0
48.00	390.0
49.00	2469.0
50.00	10761.0
51.00	3527.0
51.90	193.0
54.80	172.0
55.90	856.0
57.00	1630.0
60.00	522.0
61.00	2706.0
62.00	2744.0
63.00	2268.0
64.00	332.0
65.00	628.0
66.90	148.0
68.00	5634.0
69.00	5895.0
69.90	465.0
71.90	359.0
72.90	2699.0
74.00	9922.0
75.00	29672.0
76.00	2531.0
76.90	283.0
77.80	271.0
78.90	2113.0
79.90	577.0
80.90	2392.0
81.90	474.0
86.90	2255.0
87.90	2400.0
90.80	270.0
91.90	1836.0
92.90	2955.0
94.00	7029.0
95.00	57416.0
96.00	3788.0
96.90	143.0
103.70	259.0
105.80	270.0
115.80	248.0
116.90	426.0
117.80	228.0
118.90	305.0
127.80	216.0
128.80	187.0
129.80	210.0
134.80	120.0
140.80	719.0
142.80	855.0
144.80	218.0
147.90	190.0
149.70	104.0
154.90	130.0
157.00	181.0
170.70	134.0
171.90	824.0
173.00	881.0
173.90	55920.0
174.90	4516.0
175.90	53056.0
176.90	3560.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	536.0
37.00	2898.0
37.90	2846.0
38.90	1204.0
39.90	170.0
43.90	657.0
44.90	519.0
46.10	126.0
46.90	717.0
48.00	405.0
49.00	2658.0
50.00	11572.0
51.00	3683.0
51.90	198.0
54.90	183.0
55.90	1060.0
57.00	1737.0
57.90	106.0
60.00	648.0
61.00	2950.0
62.00	3031.0
63.00	2445.0
64.00	363.0
65.00	732.0
66.90	173.0
67.90	6085.0
69.00	6379.0
69.90	500.0
71.90	414.0
72.90	3110.0
74.00	11084.0
75.00	32416.0
76.00	2784.0
77.00	279.0
77.70	287.0
78.90	2246.0
79.90	630.0
80.90	2483.0
81.90	501.0
86.00	110.0
86.90	2441.0
87.90	2616.0
90.80	311.0
91.90	2041.0
92.90	3228.0
94.00	7729.0
95.00	63536.0
96.00	3886.0
96.90	158.0
103.70	272.0
105.90	295.0
115.90	261.0
116.90	472.0
117.80	253.0
118.90	369.0
127.80	230.0
128.80	183.0
129.80	270.0
130.90	119.0
134.80	140.0
136.80	109.0
140.80	793.0
142.80	889.0
144.90	228.0
145.80	110.0
147.90	181.0
154.90	138.0
156.90	183.0
158.80	106.0
170.70	139.0
171.90	884.0
173.00	962.0
173.90	62752.0
174.90	4960.0
175.90	59528.0
176.90	3809.0
177.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	547.0
37.00	2833.0
37.90	2810.0
38.90	1203.0
39.90	161.0
43.90	669.0
44.90	535.0
46.00	104.0
47.00	708.0
48.00	407.0
49.00	2579.0
50.00	11491.0
51.00	3511.0
52.00	194.0
54.90	175.0
55.90	1085.0
57.00	1797.0
57.90	102.0
60.00	666.0
61.00	2996.0
62.00	3030.0
62.90	2358.0
63.90	352.0
65.00	693.0
66.90	198.0
67.90	6061.0
69.00	6225.0
70.00	504.0
71.90	427.0
72.90	3146.0
74.00	11175.0
75.00	32048.0
76.00	2743.0
77.00	285.0
77.80	263.0
78.90	2145.0
79.90	624.0
80.90	2303.0
81.90	532.0
85.90	138.0
86.90	2540.0
88.00	2560.0
90.80	311.0
91.90	2077.0
92.90	3225.0
94.00	7648.0
95.00	63424.0
96.00	3804.0
96.90	144.0
103.90	256.0
105.80	311.0
115.90	266.0
116.90	496.0
117.80	231.0
118.90	413.0
128.00	231.0
128.70	155.0
129.80	272.0
130.80	123.0
134.70	122.0
136.80	118.0
140.90	793.0
142.80	899.0
144.90	216.0
145.80	132.0
147.90	162.0
155.00	157.0
156.90	168.0
158.80	121.0
170.80	132.0
171.90	894.0
173.00	995.0
173.90	63720.0
174.90	4979.0
175.90	61136.0
176.90	3752.0
177.90	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82