

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100520\
 Data File : VV018671.D
 Acq On : 05 Oct 2020 13:34
 Operator : SY/MD
 Sample : L4144-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM3

Quant Time: Oct 06 02:45:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 06 02:11:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	199860	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	203013	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	91459	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	79189	67.56	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	135.12%#
7) Chloroethane-d5	1.58	69	67518	69.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	139.34%#
11) 1,1-Dichloroethene-d2	2.12	63	122602	51.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	102.68%
21) 2-Butanone-d5	3.91	46	96361	110.21	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.21%
24) Chloroform-d	4.38	84	144107	56.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	113.72%
26) 1,2-Dichloroethane-d4	5.06	65	98996	61.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	123.04%
32) Benzene-d6	5.07	84	277973	54.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.12%
36) 1,2-Dichloropropane-d6	6.09	67	87337	56.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	112.42%
41) Toluene-d8	7.34	98	246151	50.88	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.76%
43) trans-1,3-Dichloropropene-	7.64	79	42196	50.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.54%
47) 2-Hexanone-d5	8.11	63	48198	81.67	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.67%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	88940	43.18	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.36%
64) 1,2-Dichlorobenzene-d4	11.65	152	103609	58.91	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	117.82%


Target Compounds					Ovalue
13) Acetone	2.20	43	10699	14.164 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100520\
Data File : VV018671.D
Acq On : 05 Oct 2020 13:34
Operator : SY/MD
Sample : L4144-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM3

Quant Time: Oct 06 02:45:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 06 02:11:36 2020
Response via : Initial Calibration

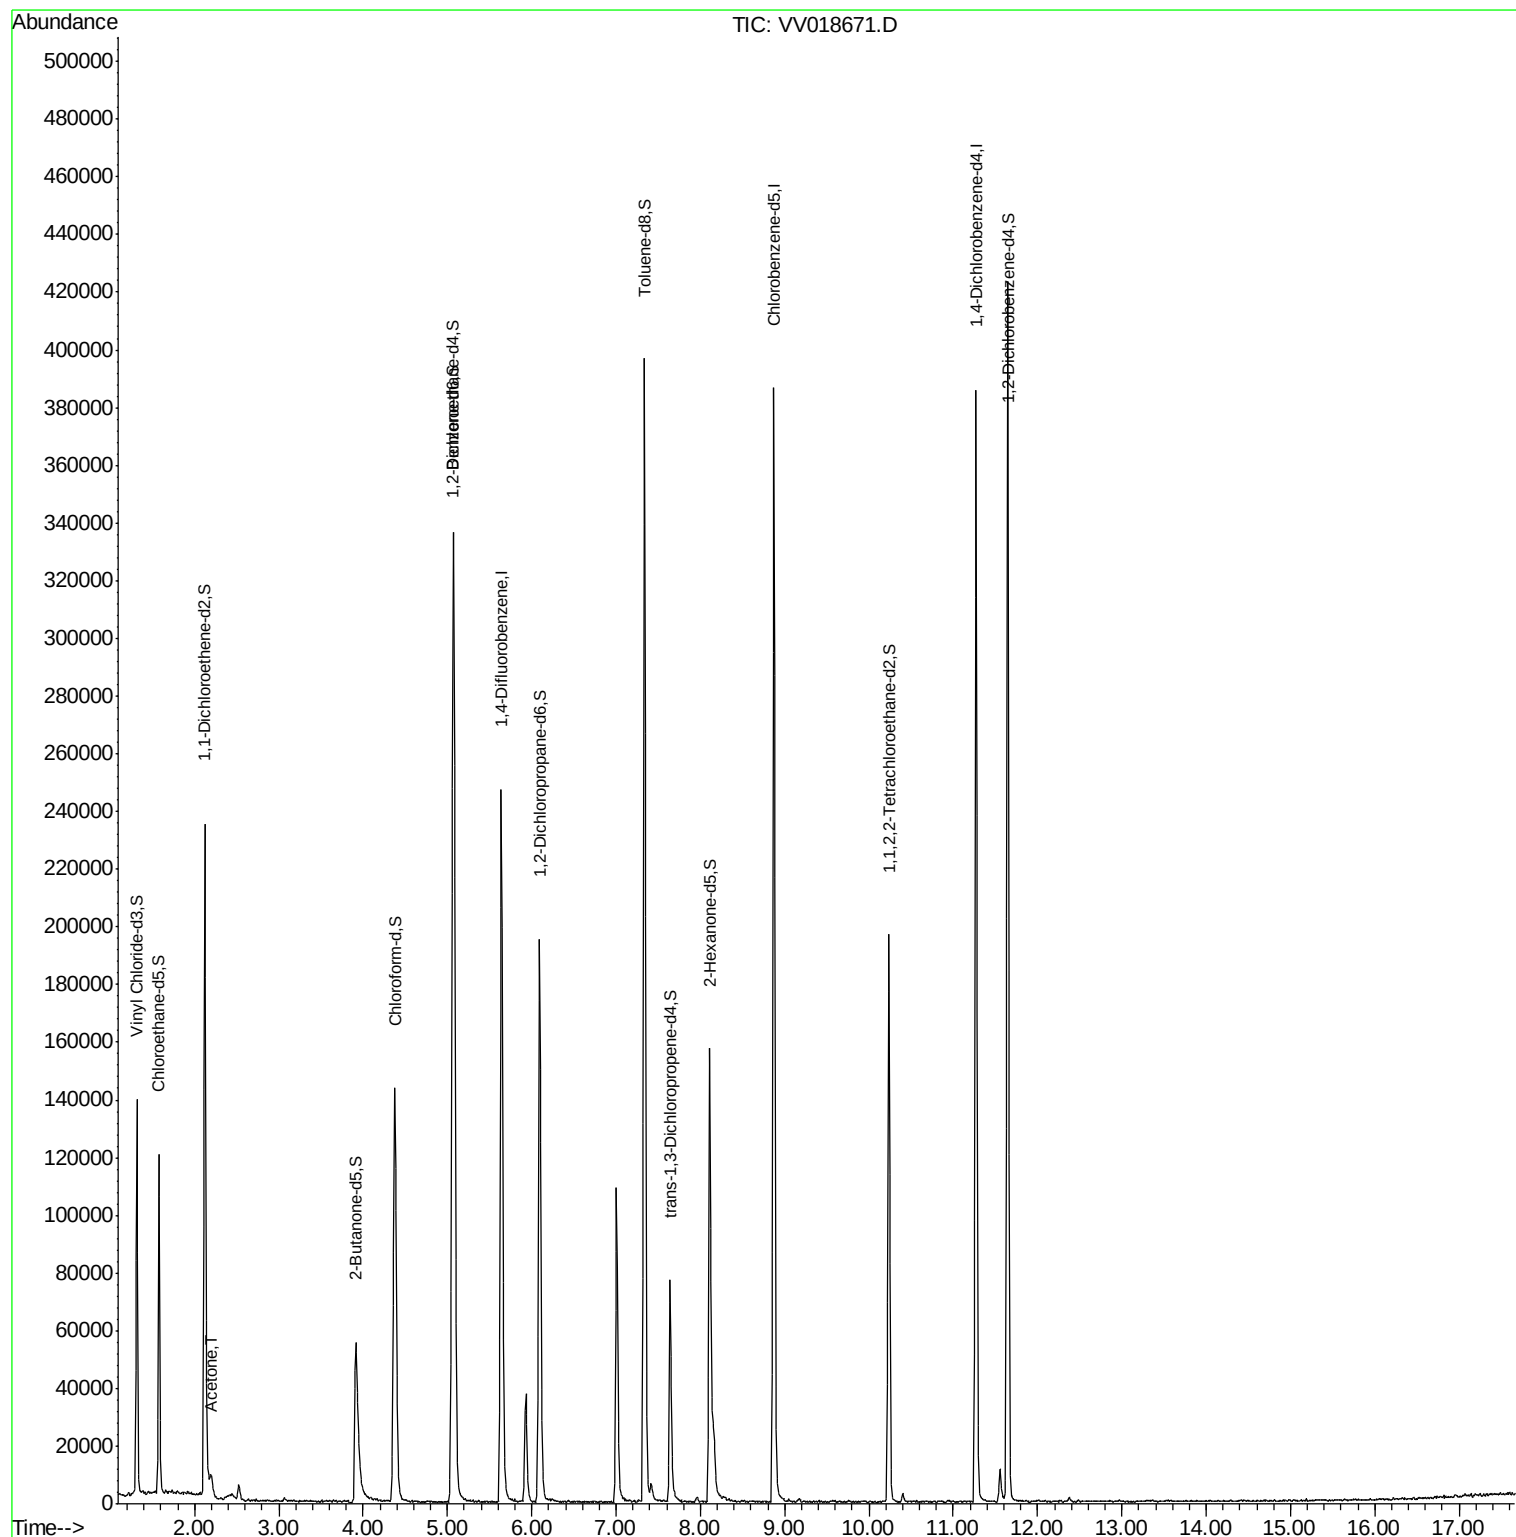

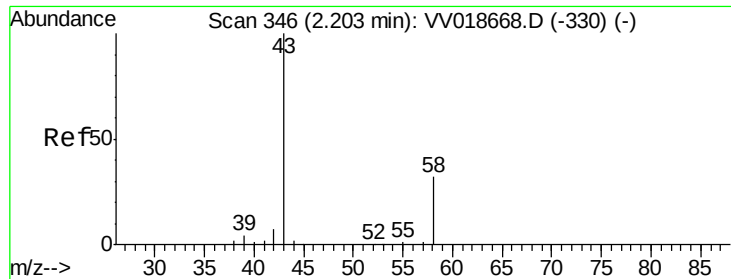

#13
Acetone
Concen: 14.164 ug/L
RT: 2.20 min Scan# 344
Delta R.T. -0.01 min
Lab File: VV018671.D
Acq: 05 Oct 2020 13:34

Instrument :
MSVOA_V
ClientSampleId :
C0AM3

Tot Ion: 43 Resp: 10699
Ion Ratio Lower Upper
43 100
58 34.7 0.0 64.0

