

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV100520\
 Data File : VV018675.D
 Acq On : 05 Oct 2020 15:34
 Operator : SY/MD
 Sample : L4254-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3S7

Quant Time: Oct 06 02:59:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 06 02:11:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	202782	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	206395	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	95099	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	73966	62.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	124.38%
7) Chloroethane-d5	1.58	69	64731	65.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	131.66%#
11) 1,1-Dichloroethene-d2	2.12	63	115656	47.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.46%
21) 2-Butanone-d5	3.91	46	94631	106.67	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.67%
24) Chloroform-d	4.38	84	141690	55.10	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.20%
26) 1,2-Dichloroethane-d4	5.06	65	98040	60.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	120.10%
32) Benzene-d6	5.07	84	265461	50.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.56%
36) 1,2-Dichloropropane-d6	6.09	67	85633	54.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.42%
41) Toluene-d8	7.34	98	236691	48.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.24%
43) trans-1,3-Dichloropropene-	7.64	79	40713	47.71	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.42%
47) 2-Hexanone-d5	8.11	63	46437	77.40	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.40%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	103834	49.58	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.16%
64) 1,2-Dichlorobenzene-d4	11.65	152	98120	53.65	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.30%


Target Compounds				Ovalue
13) Acetone	2.20	43	5607	7.316 ug/L 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV100520\
Data File : VV018675.D
Acq On : 05 Oct 2020 15:34
Operator : SY/MD
Sample : L4254-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3S7

Quant Time: Oct 06 02:59:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 06 02:11:36 2020
Response via : Initial Calibration

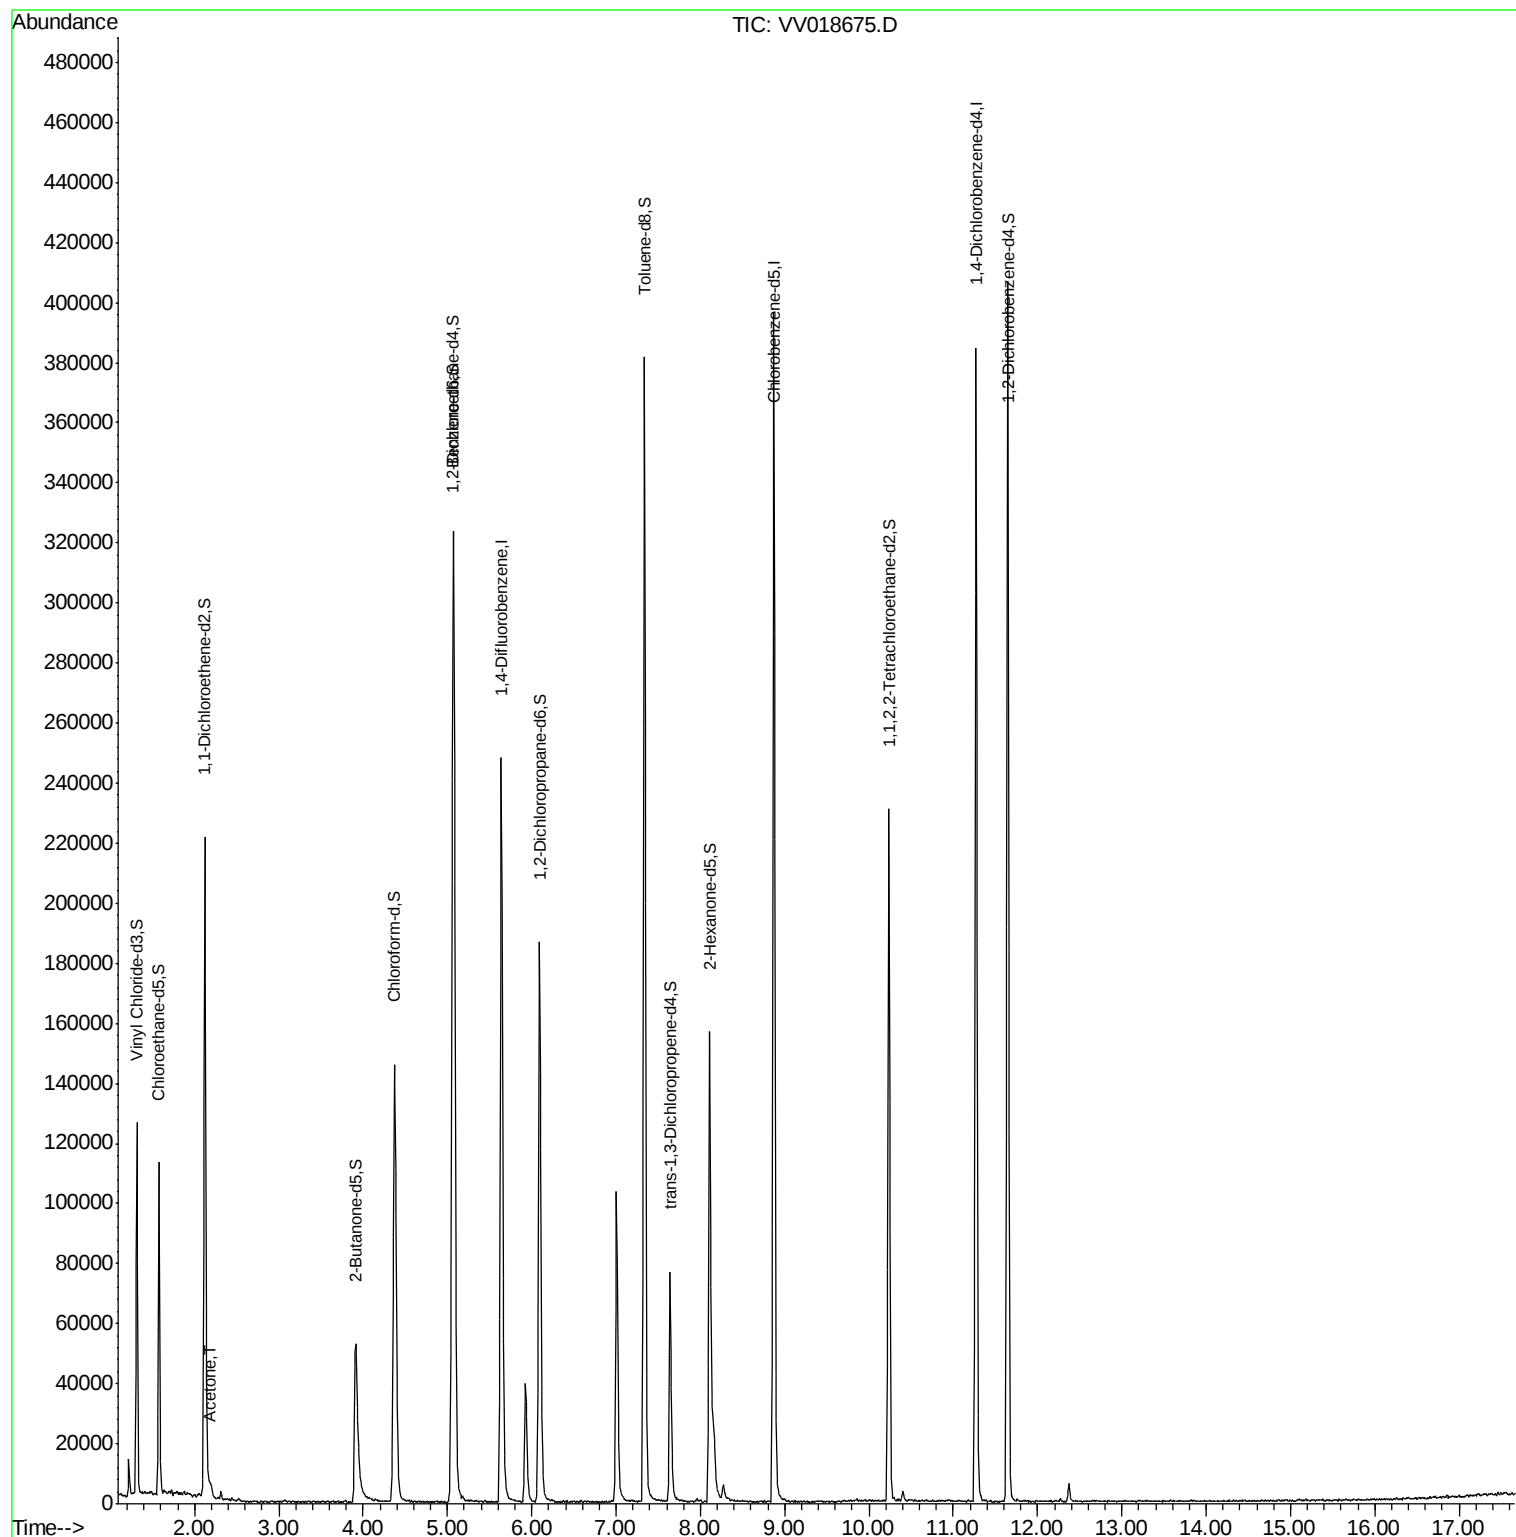

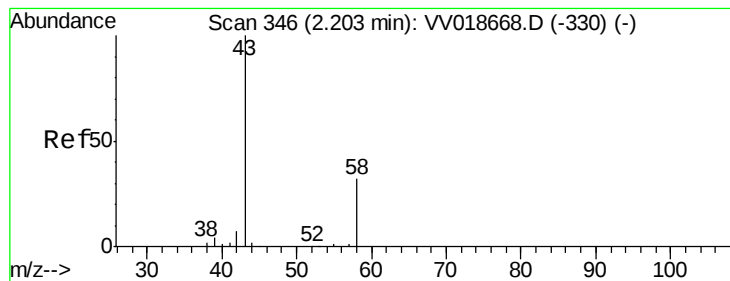

#13
 Acetone
 Concen: 7.316 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. -0.01 min
 Lab File: VV018675.D
 Acq: 05 Oct 2020 15:34

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3S7

Tot Ion: 43 Resp: 5607
 Ion Ratio Lower Upper
 43 100
 58 26.9 0.0 64.0

