


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV100520\
 Data File : VV018667.D
 Acq On : 05 Oct 2020 11:31
 Operator : SY/MD
 Sample : BFB67
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092920WMA.M
 Title : VOC Analysis
 Last Update : Tue Oct 06 02:11:36 2020

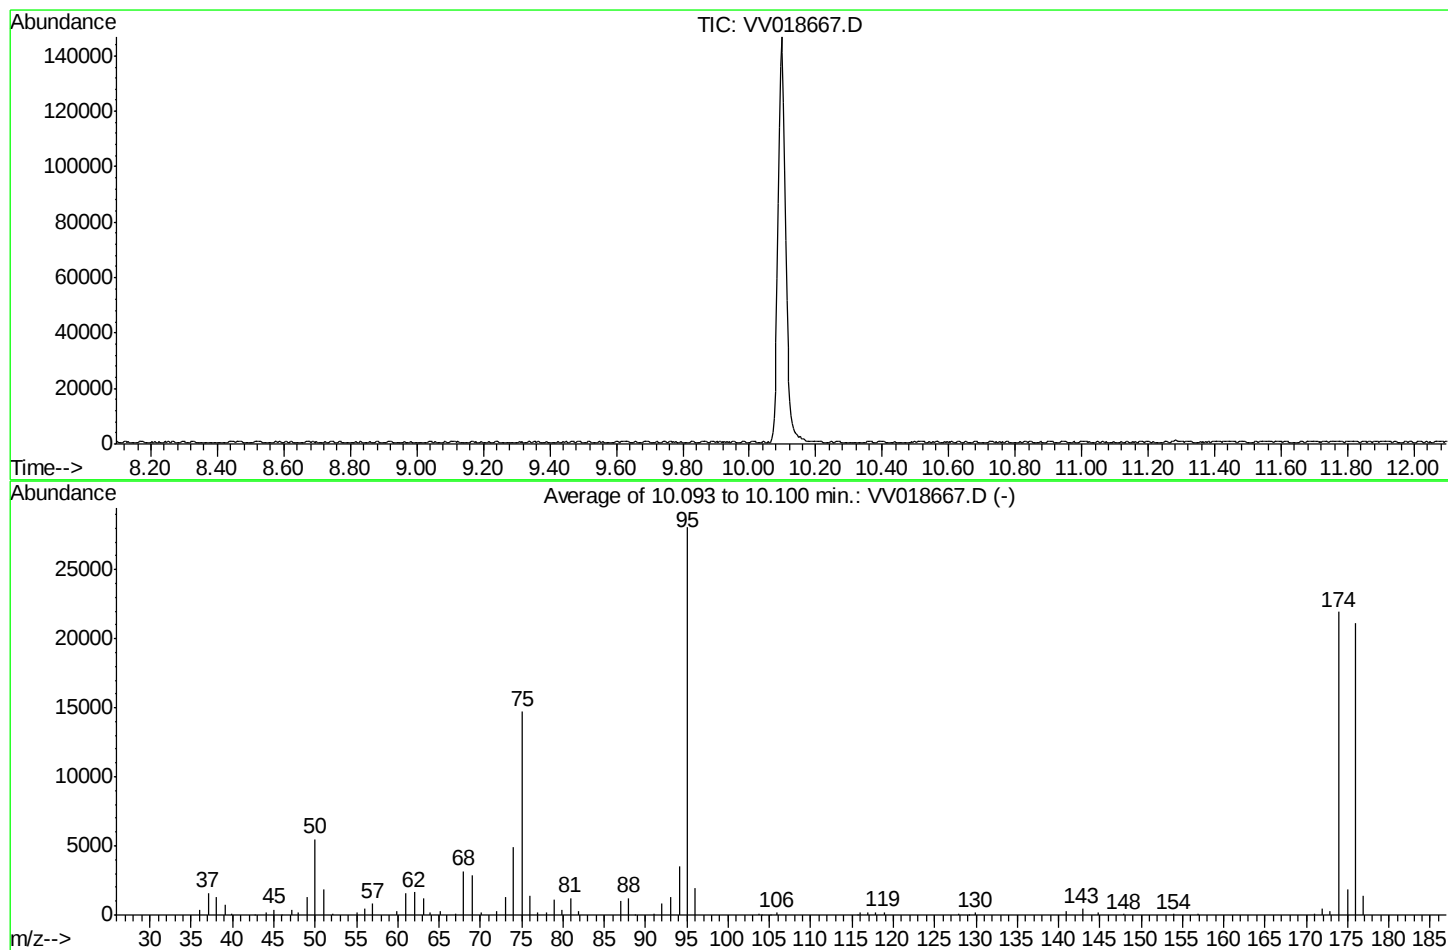

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	5495	PASS
75	95	30	80	52.5	14727	PASS
95	95	100	100	100.0	28053	PASS
96	95	5	9	7.1	1988	PASS
173	174	0.00	2	1.2	263	PASS
174	95	50	120	78.2	21946	PASS
175	174	5	9	8.4	1849	PASS
176	174	95	101	96.4	21162	PASS
177	176	5	9	6.4	1363	PASS

m/z	Abundance
36.00	397.0
37.00	1484.0
38.10	1347.0
39.00	671.0
40.00	183.0
44.00	698.0
45.10	342.0
47.10	447.0
47.90	210.0
49.00	1211.0
50.00	5339.0
51.10	1973.0
52.20	203.0
54.90	186.0
56.00	493.0
57.00	732.0
59.90	324.0
61.00	1480.0
62.00	1612.0
63.10	1073.0
63.90	156.0
65.10	352.0
68.00	3005.0
69.10	2832.0
70.10	179.0
72.00	225.0
73.00	1212.0
74.00	4746.0
75.10	14205.0
76.00	1305.0
77.00	184.0
78.00	148.0
78.90	1071.0
79.90	397.0
80.90	1257.0
82.00	343.0
86.90	1098.0
87.90	1299.0
91.00	147.0
92.00	797.0
93.00	1254.0
94.10	3400.0
95.10	27352.0
96.00	2086.0
103.80	178.0
105.90	177.0
115.60	102.0
116.00	137.0
116.90	216.0
117.80	153.0
118.90	236.0
129.90	120.0
140.90	279.0
142.90	480.0
144.90	147.0
148.00	107.0
170.90	106.0
171.90	394.0
172.90	380.0
174.00	20864.0
175.00	1689.0
176.00	19736.0
176.90	1330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	387.0
37.10	1663.0
38.10	1290.0
39.10	768.0
39.90	220.0
42.70	102.0
44.00	727.0
45.10	398.0
47.10	402.0
48.00	223.0
49.10	1288.0
50.00	5695.0
51.10	1985.0
52.10	133.0
55.00	206.0
56.00	467.0
57.00	846.0
59.80	321.0
61.00	1642.0
62.00	1713.0
63.10	1225.0
63.90	135.0
65.10	321.0
67.00	111.0
68.00	3282.0
69.10	2925.0
70.00	220.0
72.00	274.0
73.00	1337.0
74.00	5057.0
75.10	15264.0
76.00	1428.0
76.90	207.0
78.10	134.0
78.90	1135.0
79.90	421.0
80.90	1261.0
82.00	331.0
86.90	1073.0
88.00	1248.0
91.00	145.0
92.00	782.0
93.00	1327.0
94.10	3617.0
95.10	29240.0
96.00	2040.0
103.80	166.0
105.90	169.0
116.00	159.0
116.90	223.0
117.80	152.0
118.80	231.0
127.90	110.0
130.00	166.0
141.00	313.0
142.90	483.0
144.90	160.0
147.90	106.0
154.00	122.0
156.90	104.0
171.00	110.0
171.90	507.0
172.90	411.0
174.00	22864.0
175.00	1869.0
176.00	21960.0
177.00	1432.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.90	380.0
37.10	1640.0
38.10	1249.0
39.00	772.0
39.90	235.0
44.00	731.0
45.00	417.0
46.00	105.0
47.10	313.0
48.00	223.0
49.10	1312.0
50.00	5452.0
51.10	1744.0
55.10	204.0
56.00	426.0
57.00	892.0
59.90	294.0
61.00	1571.0
62.00	1618.0
63.10	1289.0
63.90	139.0
65.10	279.0
66.90	105.0
68.00	3198.0
69.00	2800.0
70.00	240.0
72.00	291.0
73.00	1313.0
74.00	4889.0
75.10	14714.0
76.00	1379.0
76.90	198.0
78.10	150.0
78.90	1103.0
79.90	376.0
80.90	1141.0
81.90	286.0
87.00	899.0
88.00	1158.0
88.70	101.0
91.00	128.0
92.00	804.0
93.00	1302.0
94.10	3469.0
95.10	27568.0
96.00	1840.0
104.00	143.0
105.10	105.0
106.00	151.0
116.00	138.0
117.00	231.0
117.80	139.0
118.80	230.0
127.90	129.0
129.10	114.0
130.00	188.0
141.00	336.0
142.90	419.0
144.80	160.0
154.00	130.0
156.90	103.0
171.00	104.0
171.90	533.0
174.00	22112.0
175.00	1991.0
176.00	21792.0
177.00	1328.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

Scan 2789 (10.058 min): VV018667.D
BFB67

m/z	Abundance
39.70	108.0
40.00	111.0
44.00	500.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67