
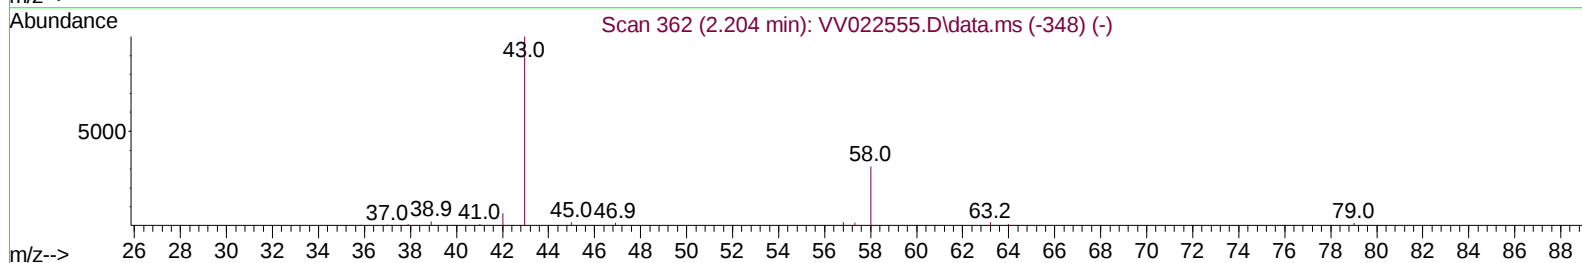
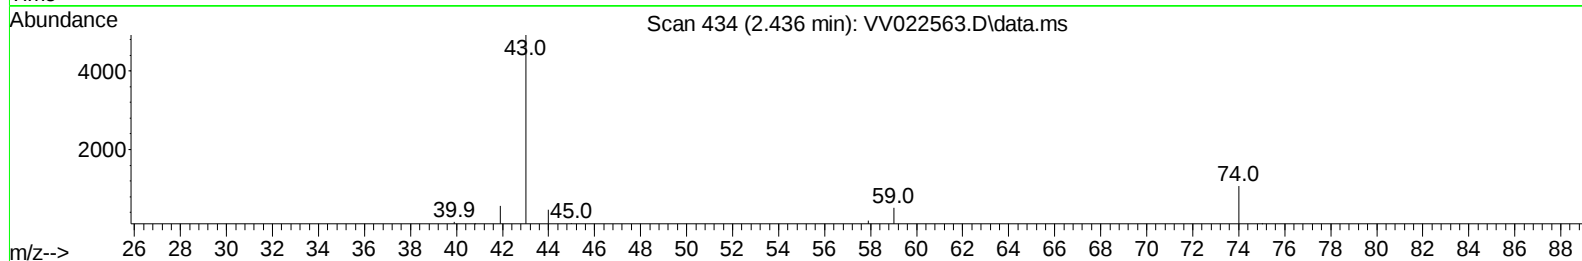


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022563.D
Acq On : 05 Oct 2021 09:45
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 06 05:18:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 05 01:58:14 2021
Response via : Initial Calibration

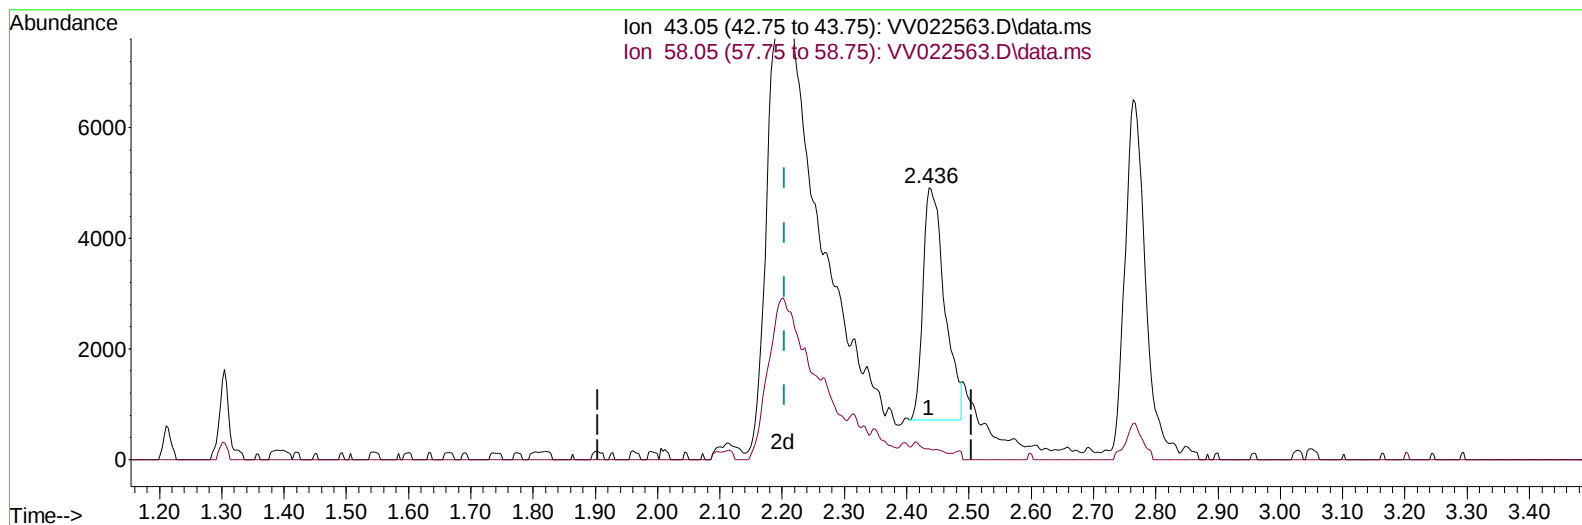

TIC: VV022563.D\data.ms

(13) Acetone (T)




2.436min (+ 0.232) 8.91 ug/L

response 10139

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	10.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022563.D
 Acq On : 05 Oct 2021 09:45
 Operator : SY/MD
 Sample : VSTDCCC005
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 06 05:18:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 05 01:58:14 2021
 Response via : Initial Calibration

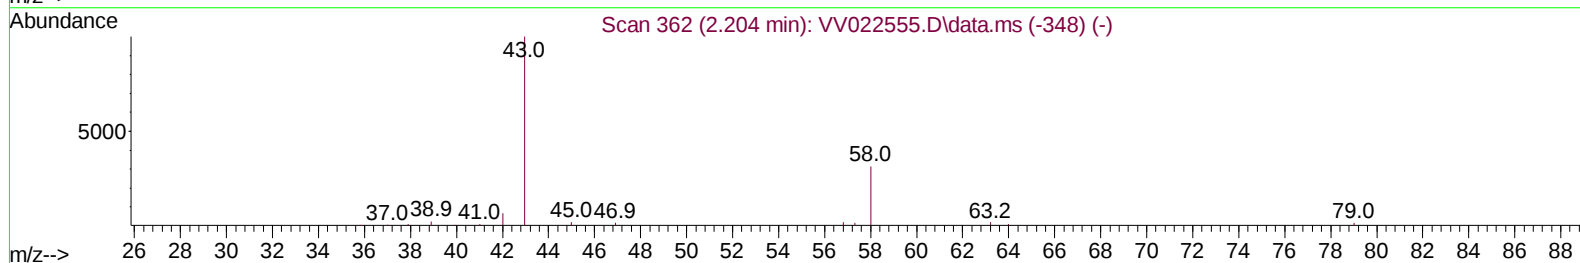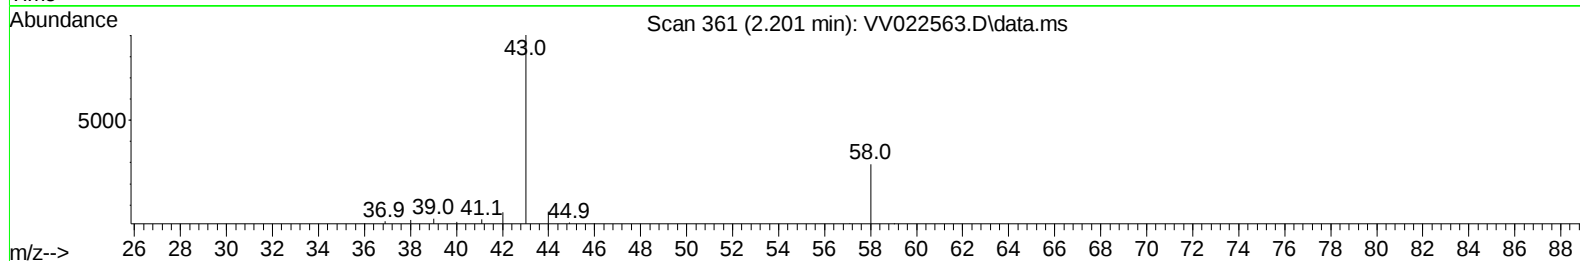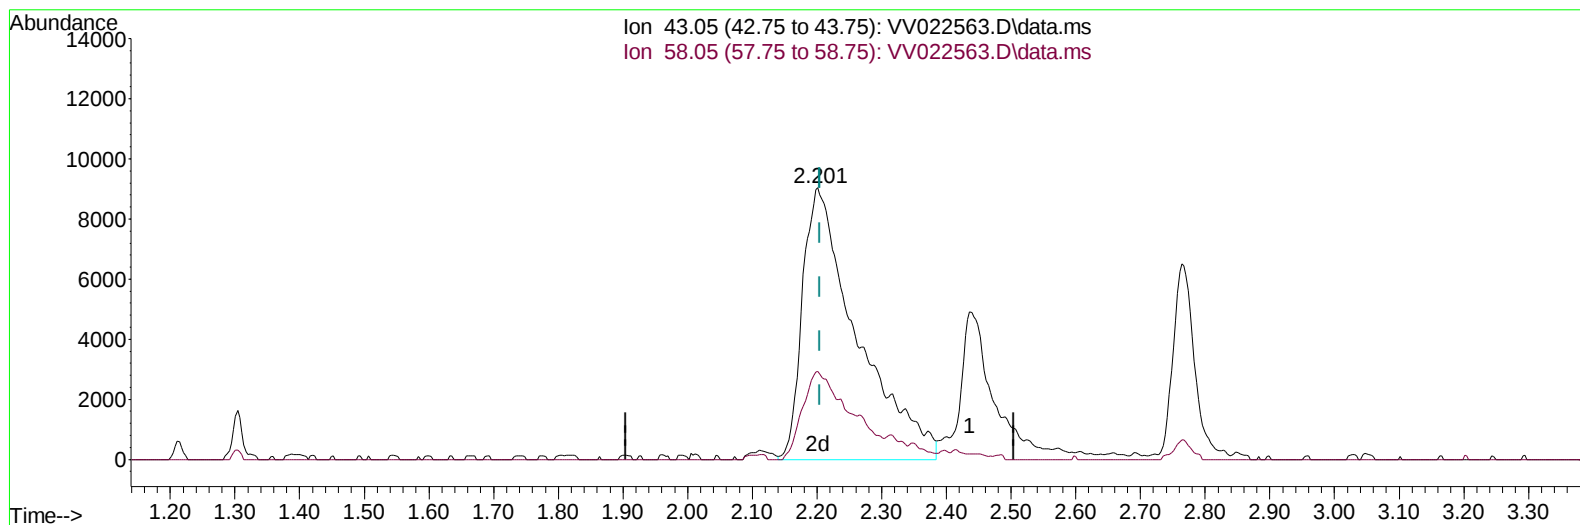

TIC: VV022563.D\data.ms

(13) Acetone (T)

2.201min (-0.003) 46.38 ug/L m

response 52766

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	1.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022563.D
 Acq On : 05 Oct 2021 09:45
 Operator : SY/MD
 Sample : VSTDCCC005
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 06 05:18:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 05 01:58:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	111694	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	106997	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59437	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	17211	4.809	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	96.200%	
7) Chloroethane-d5	1.565	69	24846	5.151	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	103.000%	
11) 1,1-Dichloroethene-d2	2.105	63	52570	5.063	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	101.200%	
20) 2-Butanone-d5	3.905	46	82852	39.166	ug/L	-0.03
Spiked Amount 50.000	Range 40	- 130	Recovery	=	78.340%	
24) Chloroform-d	4.346	84	63249	4.590	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.800%	
26) 1,2-Dichloroethane-d4	5.027	65	30715	4.732	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	94.600%	
32) Benzene-d6	5.047	84	113633	4.713	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.200%	
36) 1,2-Dichloropropane-d6	6.066	67	35702	4.197	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	84.000%	
41) Toluene-d8	7.314	98	100118	4.953	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.000%	
43) trans-1,3-Dichloroprop...	7.622	79	10217	4.538	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	90.800%	
46) 2-Hexanone-d5	8.088	63	66631	47.802	ug/L	-0.01
Spiked Amount 50.000	Range 45	- 130	Recovery	=	95.600%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29592	4.578	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	91.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	42373	4.609	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	92.200%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.127	85	44238	5.200	ug/L	98
3) Chloromethane	1.237	50	45344	5.324	ug/L	100
5) Vinyl chloride	1.307	62	45650	5.310	ug/L	99
6) Bromomethane	1.516	94	29689	5.203	ug/L	99
8) Chloroethane	1.581	64	27628	5.053	ug/L	100
9) Trichlorofluoromethane	1.748	101	68175	5.301	ug/L	99
10) 1,1,2-Trichloro-1,2,2-...	2.111	101	38140	5.158	ug/L	97
12) 1,1-Dichloroethene	2.114	96	37030	5.412	ug/L	97
13) Acetone	2.201	43	52766m	46.384	ug/L	
14) Carbon disulfide	2.288	76	109103	5.451	ug/L	98
15) Methyl Acetate	2.436	43	11366	3.393	ug/L #	68
16) Methylene chloride	2.503	84	40318	5.114	ug/L	95
17) Methyl tert-butyl Ether	2.767	73	80266	4.616	ug/L	97
18) trans-1,2-Dichloroethene	2.754	96	37807	5.070	ug/L	99
19) 1,1-Dichloroethane	3.185	63	65625	4.905	ug/L	99
21) 2-Butanone	3.992	43	77680	42.655	ug/L	87
22) cis-1,2-Dichloroethene	3.905	96	37979	4.694	ug/L	97
23) Bromochloromethane	4.246	128	18520	4.863	ug/L	89

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022563.D
 Acq On : 05 Oct 2021 09:45
 Operator : SY/MD
 Sample : VSTDCCC005
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 06 05:18:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 05 01:58:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
25) Chloroform	4.372	83	72029	4.931	ug/L	97
27) 1,2-Dichloroethane	5.130	62	37387	4.809	ug/L	96
29) 1,1,1-Trichloroethane	4.603	97	61031	4.993	ug/L	98
30) Cyclohexane	4.674	56	53253	4.808	ug/L	100
31) Carbon tetrachloride	4.822	117	53879	4.968	ug/L	99
33) Benzene	5.095	78	141837	4.919	ug/L	100
34) Trichloroethene	5.912	95	39801	4.750	ug/L	97
35) Methylcyclohexane	6.127	83	55914	4.762	ug/L	98
37) 1,2-Dichloropropane	6.172	63	34407	4.888	ug/L	100
38) Bromodichloromethane	6.506	83	43524	4.879	ug/L	97
39) cis-1,3-Dichloropropene	7.027	75	43518	4.587	ug/L	96
40) 4-Methyl-2-pentanone	7.227	43	195254	50.390	ug/L	99
42) Toluene	7.387	91	157789	5.209	ug/L	99
44) trans-1,3-Dichloropropene	7.651	75	37440	4.727	ug/L	100
45) 1,1,2-Trichloroethane	7.838	97	25977	4.943	ug/L	98
47) Tetrachloroethene	7.973	164	33048	5.072	ug/L	98
48) 2-Hexanone	8.140	43	142036	50.952	ug/L	98
49) Dibromochloromethane	8.246	129	32695	5.278	ug/L	99
50) 1,2-Dibromoethane	8.352	107	24748	5.066	ug/L	93
51) Chlorobenzene	8.883	112	101612	5.125	ug/L	98
52) Ethylbenzene	9.011	91	160714	5.170	ug/L	100
53) m,p-xylene	9.140	106	64637	5.454	ug/L	93
54) o-xylene	9.545	106	61247	5.194	ug/L	98
55) Styrene	9.561	104	106288	5.302	ug/L	100
57) 1,1,2,2-Tetrachloroethane	10.243	83	27758	4.868	ug/L	100
59) Bromoform	9.731	173	17746	5.089	ug/L	98
60) Isopropylbenzene	9.931	105	164087	5.135	ug/L	100
61) 1,2,3-Trichloropropane	10.275	75	20953	4.756	ug/L	95
62) 1,3,5-Trimethylbenzene	10.538	105	131398	5.072	ug/L	100
63) 1,2,4-Trimethylbenzene	10.915	105	135074	5.132	ug/L	100
64) 1,3-Dichlorobenzene	11.182	146	84217	5.148	ug/L	96
65) 1,4-Dichlorobenzene	11.275	146	83484	4.989	ug/L	98
67) 1,2-Dichlorobenzene	11.645	146	76667	5.030	ug/L	97
68) 1,2-Dibromo-3-chloropr...	12.429	75	3785	4.495	ug/L	88
69) 1,3,5-Trichlorobenzene	12.648	180	61710	5.039	ug/L	100
70) 1,2,4-trichlorobenzene	13.262	180	49614	5.048	ug/L	99
71) Naphthalene	13.503	128	78271	4.860	ug/L	99
72) 1,2,3-Trichlorobenzene	13.744	180	46616	5.161	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Abundance

TIC: VV022563.D\data.ms

Time-->

360000

340000

320000

300000

280000

260000

240000

220000

200000

180000

160000

140000

120000

100000

80000

60000

40000

20000

0

2.00

3.00

4.00

5.00

6.00

7.00

8.00

9.00

10.00

11.00

12.00

13.00

14.00

15.00

16.00

17.00

1,1-Dichloroethane, T

1,1,1-Trichloroethane, T

1,1,2-Trichloroethane, T

1,2-Dichloroethane, T

1,2,3-Trichloroethane, T

1,2,4-Trichloroethane, T

1,2,5-Trichloroethane, T

1,2,6-Trichloroethane, T

1,2,7-Trichloroethane, T

1,2,8-Trichloroethane, T

1,2,9-Trichloroethane, T

1,2,10-Trichloroethane, T

1,2,11-Trichloroethane, T

1,2,12-Trichloroethane, T

1,2,13-Trichloroethane, T

1,2,14-Trichloroethane, T

1,2,15-Trichloroethane, T

1,2,16-Trichloroethane, T

1,2,17-Trichloroethane, T

1,2,18-Trichloroethane, T

1,2,19-Trichloroethane, T

1,2,20-Trichloroethane, T

1,2,21-Trichloroethane, T

1,2,22-Trichloroethane, T

1,2,23-Trichloroethane, T

1,2,24-Trichloroethane, T

1,2,25-Trichloroethane, T

1,2,26-Trichloroethane, T

1,2,27-Trichloroethane, T

1,2,28-Trichloroethane, T

1,2,29-Trichloroethane, T

1,2,30-Trichloroethane, T

1,2,31-Trichloroethane, T

1,2,32-Trichloroethane, T

1,2,33-Trichloroethane, T

1,2,34-Trichloroethane, T

1,2,35-Trichloroethane, T

1,2,36-Trichloroethane, T

1,2,37-Trichloroethane, T

1,2,38-Trichloroethane, T

1,2,39-Trichloroethane, T

1,2,40-Trichloroethane, T

1,2,41-Trichloroethane, T

1,2,42-Trichloroethane, T

1,2,43-Trichloroethane, T

1,2,44-Trichloroethane, T

1,2,45-Trichloroethane, T

1,2,46-Trichloroethane, T

1,2,47-Trichloroethane, T

1,2,48-Trichloroethane, T

1,2,49-Trichloroethane, T

1,2,50-Trichloroethane, T

1,2,51-Trichloroethane, T

1,2,52-Trichloroethane, T

1,2,53-Trichloroethane, T

1,2,54-Trichloroethane, T

1,2,55-Trichloroethane, T

1,2,56-Trichloroethane, T

1,2,57-Trichloroethane, T

1,2,58-Trichloroethane, T

1,2,59-Trichloroethane, T

1,2,60-Trichloroethane, T

1,2,61-Trichloroethane, T

1,2,62-Trichloroethane, T

1,2,63-Trichloroethane, T

1,2,64-Trichloroethane, T

1,2,65-Trichloroethane, T

1,2,66-Trichloroethane, T

1,2,67-Trichloroethane, T

1,2,68-Trichloroethane, T

1,2,69-Trichloroethane, T

1,2,70-Trichloroethane, T

1,2,71-Trichloroethane, T

1,2,72-Trichloroethane, T

1,2,73-Trichloroethane, T

1,2,74-Trichloroethane, T

1,2,75-Trichloroethane, T

1,2,76-Trichloroethane, T

1,2,77-Trichloroethane, T

1,2,78-Trichloroethane, T

1,2,79-Trichloroethane, T

1,2,80-Trichloroethane, T

1,2,81-Trichloroethane, T

1,2,82-Trichloroethane, T

1,2,83-Trichloroethane, T

1,2,84-Trichloroethane, T

1,2,85-Trichloroethane, T

1,2,86-Trichloroethane, T

1,2,87-Trichloroethane, T

1,2,88-Trichloroethane, T

1,2,89-Trichloroethane, T

1,2,90-Trichloroethane, T

1,2,91-Trichloroethane, T

1,2,92-Trichloroethane, T

1,2,93-Trichloroethane, T

1,2,94-Trichloroethane, T

1,2,95-Trichloroethane, T

1,2,96-Trichloroethane, T

1,2,97-Trichloroethane, T

1,2,98-Trichloroethane, T

1,2,99-Trichloroethane, T

1,3-Dichlorobenzene, T

1,3,5-Dichlorobenzene, T

1,3,5-Trichlorobenzene

1,2,4-trichlorobenzene, T

1,2,3-Trichlorobenzene, T

Naphthalene

1,2-Dibromo-3-chloropropane, T

Bromoform, T

1,2,3,4,5-Pentachlorobenzene, T

1,2,3,4,5,6-Hexachlorobenzene, T

1,2,3,4,5,6,7-Heptachlorobenzene, T

1,2,3,4,5,6,7,8-Octachlorobenzene, T

1,2,3,4,5,6,7,8,9-Nonachlorobenzene, T

1,2,3,4,5,6,7,8,9,10-Decachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11-Undecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12-Dodecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13-Tridecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14-Tetradecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15-Pentadecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16-Hexadecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17-Heptadecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18-Octadecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19-Nonadecachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20-Eicetachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21-Hentriacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22-Tricacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23-Tetracacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24-Pentacacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24,25-Hexacacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24,25,26-Heptacacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24,25,26,27-Octacacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24,25,26,27,28-Nonacacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24,25,26,27,28,29-Decacacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24,25,26,27,28,29,30-Undecacacachlorobenzene, T

1,2,3,4,5,6,7,8,9,10,11,12,13,14,15,16,17,18,19,20,21,22,23,24,25,26,27,28,29,30,31-Dodecacacachlorobenzene, T

1,2