




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022599.D
 Acq On : 06 Oct 2021 03:49
 Operator : SY/MD
 Sample : M4050-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C0

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:36 AM

Quant Time: Oct 06 08:09:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

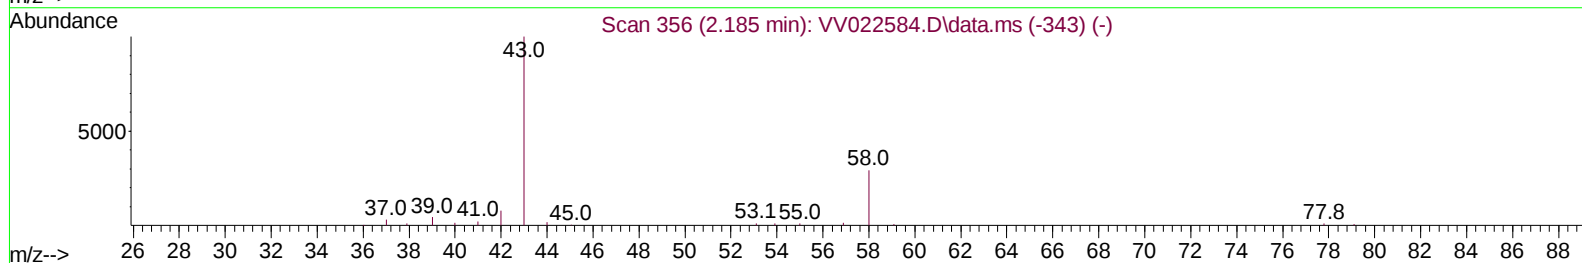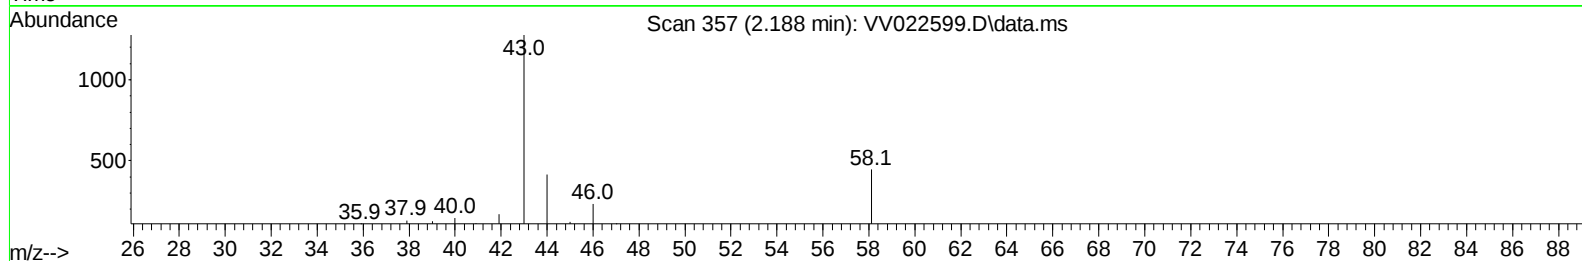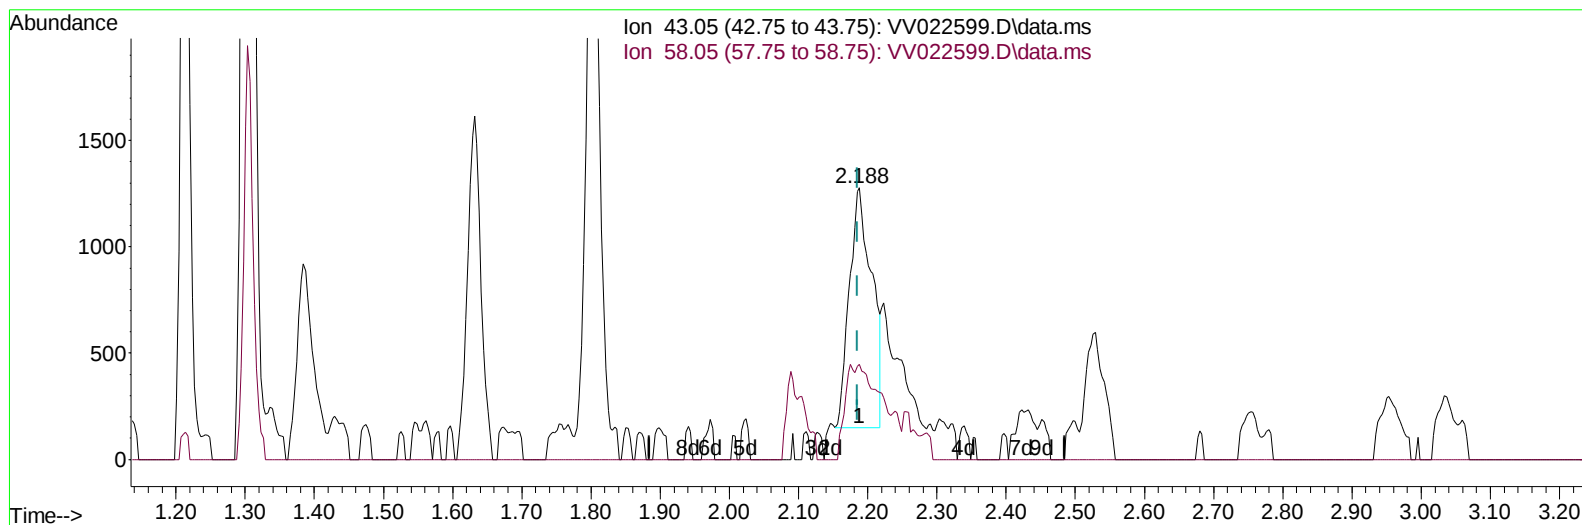

TIC: VV022599.D\data.ms

(13) Acetone (T)

2.188min (+ 0.003) 2.42 ug/L

response 2524

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	18.86#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022599.D
 Acq On : 06 Oct 2021 03:49
 Operator : SY/MD
 Sample : M4050-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C0

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:36 AM

Quant Time: Oct 06 08:09:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

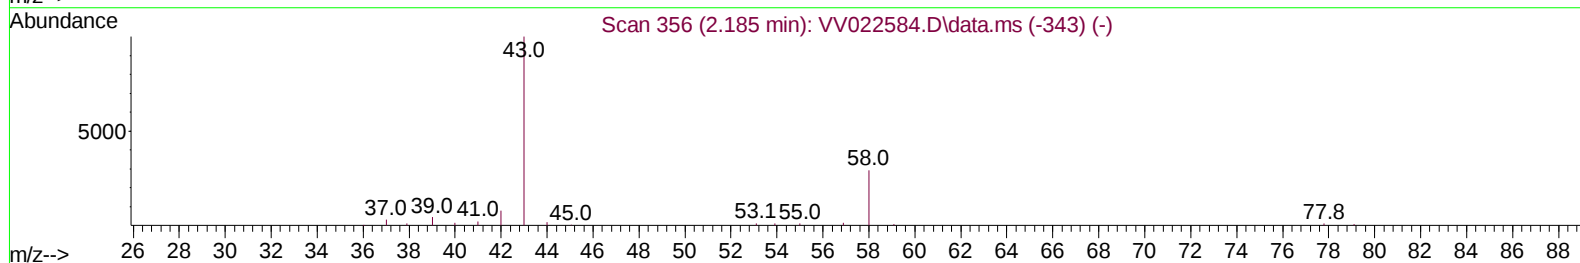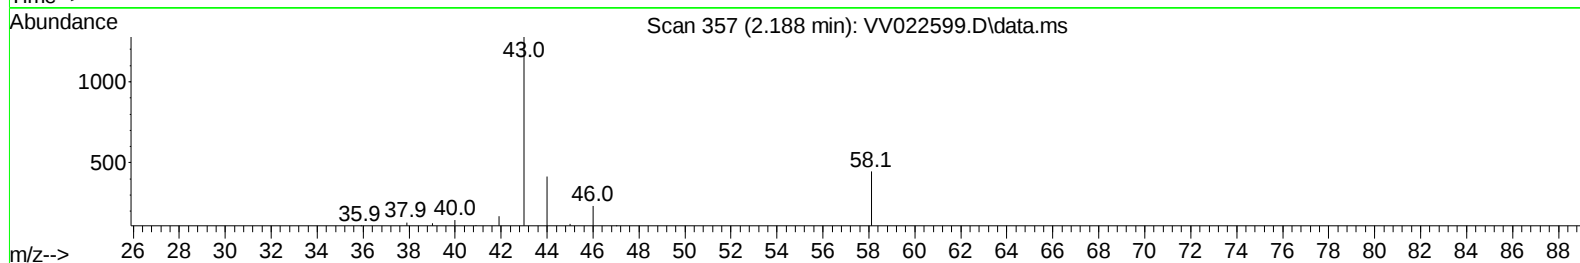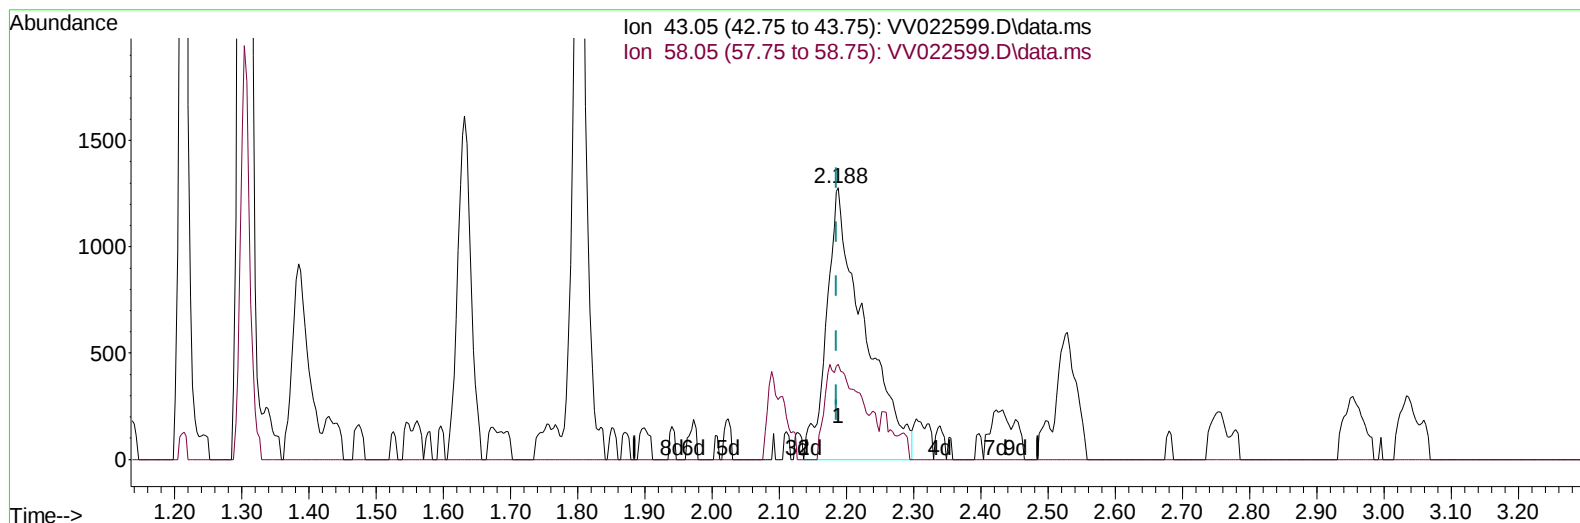

TIC: VV022599.D\data.ms

(13) Acetone (T)

2.188min (+ 0.003) 4.77 ug/L m

response 4983

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	9.55
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022599.D
Acq On : 06 Oct 2021 03:49
Operator : SY/MD
Sample : M4050-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C0

Manual Integrations
APPROVED

MMDadoda
10/7/2021 9:33:36 AM

Quant Time: Oct 06 08:09:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 07:50:25 2021
Response via : Initial Calibration

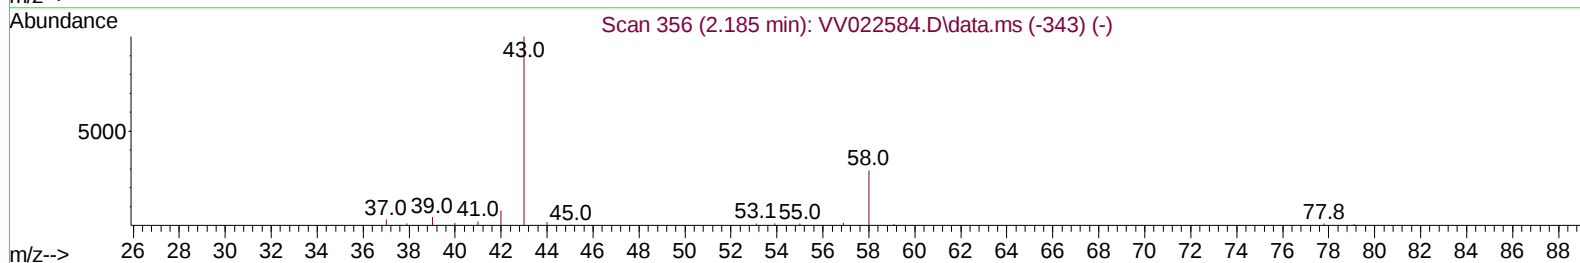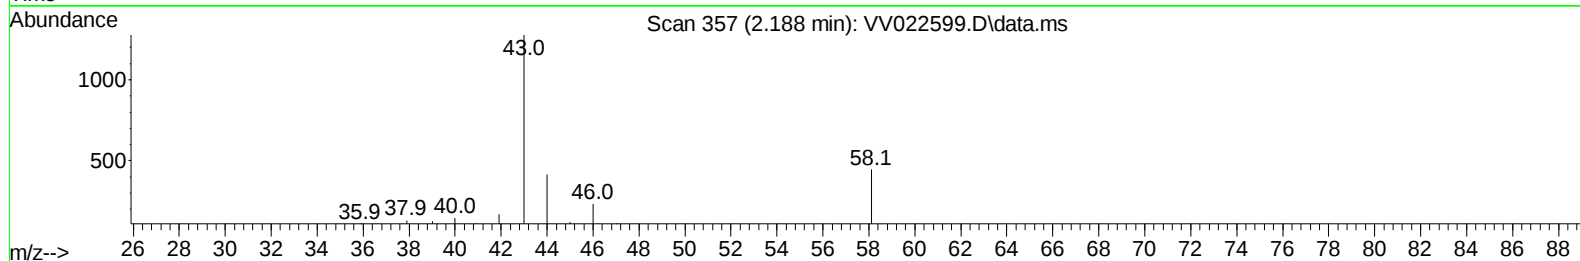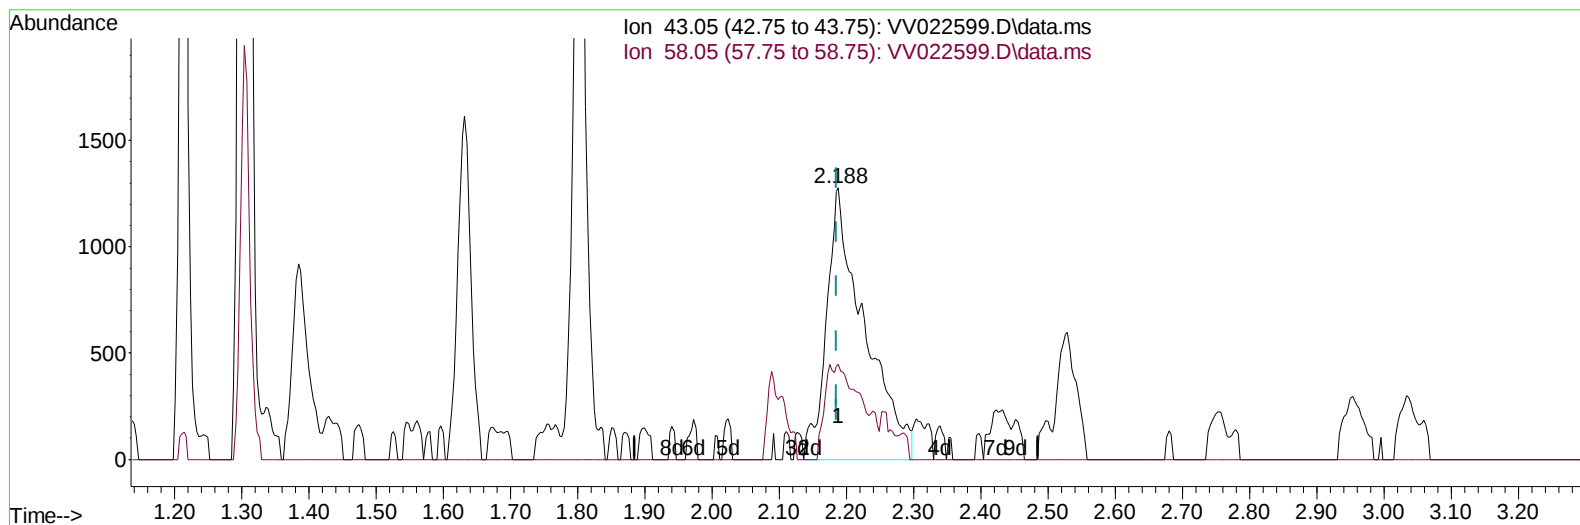

TIC: VV022599.D\data.ms

(13) Acetone (T)

2.188min (+ 0.003) 4.77 ug/L m

response 4983

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	9.55
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022599.D
 Acq On : 06 Oct 2021 03:49
 Operator : SY/MD
 Sample : M4050-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C0

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:36 AM

Quant Time: Oct 06 08:09:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	102481	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	100155	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	45395	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	15581	4.745	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	95.000%		
7) Chloroethane-d5	1.564	69	24017	5.426	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	108.600%		
11) 1,1-Dichloroethene-d2	2.104	63	31499	3.306	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	66.200%		
20) 2-Butanone-d5	3.899	46	96714	49.829	ug/L	-0.01
Spiked Amount 50.000	Range 40 - 130		Recovery =	99.660%		
24) Chloroform-d	4.349	84	56634	4.479	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.600%		
26) 1,2-Dichloroethane-d4	5.037	65	29250	4.911	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.200%		
32) Benzene-d6	5.050	84	102831	4.556	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	91.200%		
36) 1,2-Dichloropropane-d6	6.072	67	35050	4.402	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	88.000%		
41) Toluene-d8	7.320	98	78651	4.157	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	83.200%		
43) trans-1,3-Dichloroprop...	7.628	79	8673	4.116	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	82.400%		
46) 2-Hexanone-d5	8.091	63	66315	50.825	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	101.660%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	28232	4.666	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	93.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	35532	5.060	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	101.200%		
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.108	96	543	0.086	ug/L #	1
13) Acetone	2.188	43	4983m	4.774	ug/L	
14) Carbon disulfide	2.291	76	1723	0.094	ug/L	95
22) cis-1,2-Dichloroethene	3.911	96	6716	0.905	ug/L	100
34) Trichloroethene	5.921	95	5640	0.719	ug/L	98
42) Toluene	7.397	91	5942	0.210	ug/L	92
53) m,p-xylene	9.146	106	1441	0.130	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022599.D
Acq On : 06 Oct 2021 03:49
Operator : SY/MD
Sample : M4050-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C0

Manual Integrations
APPROVED

MMDadoda
10/7/2021 9:33:36 AM

Quant Time: Oct 06 08:09:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 07:50:25 2021
Response via : Initial Calibration

