




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022603.D
 Acq On : 06 Oct 2021 05:26
 Operator : SY/MD
 Sample : M4050-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C4

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:43 AM

Quant Time: Oct 06 08:10:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

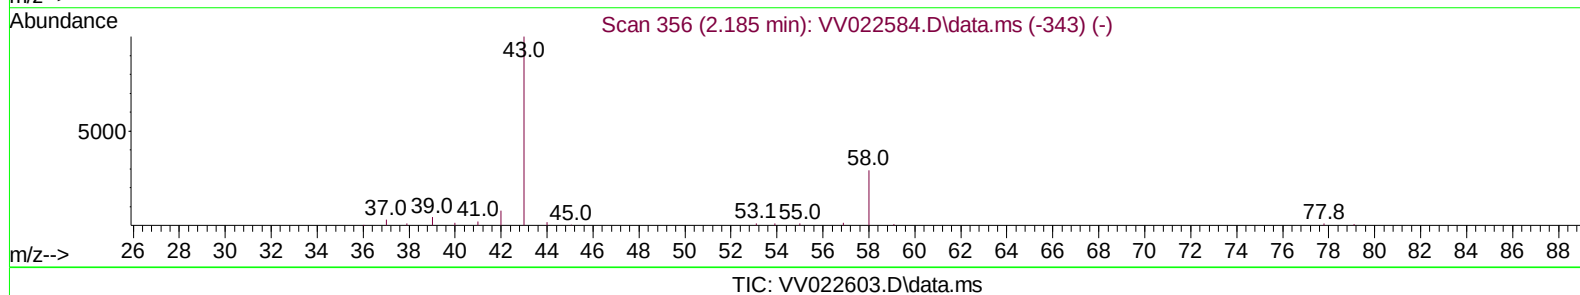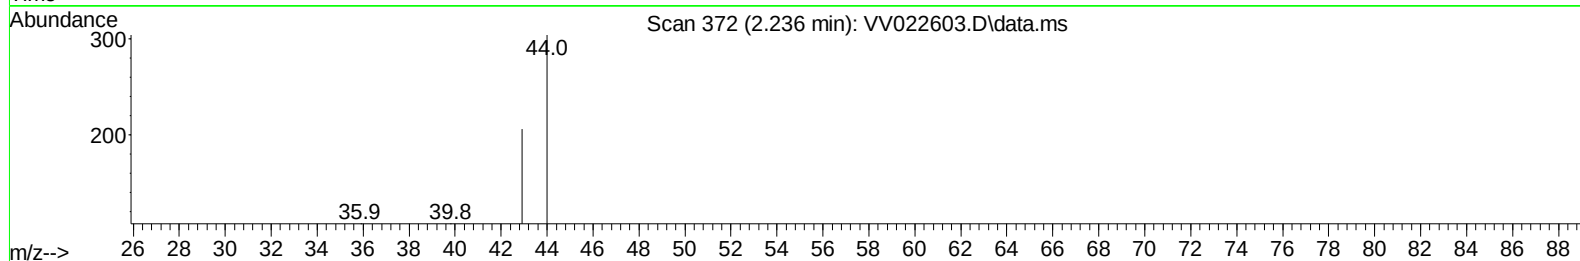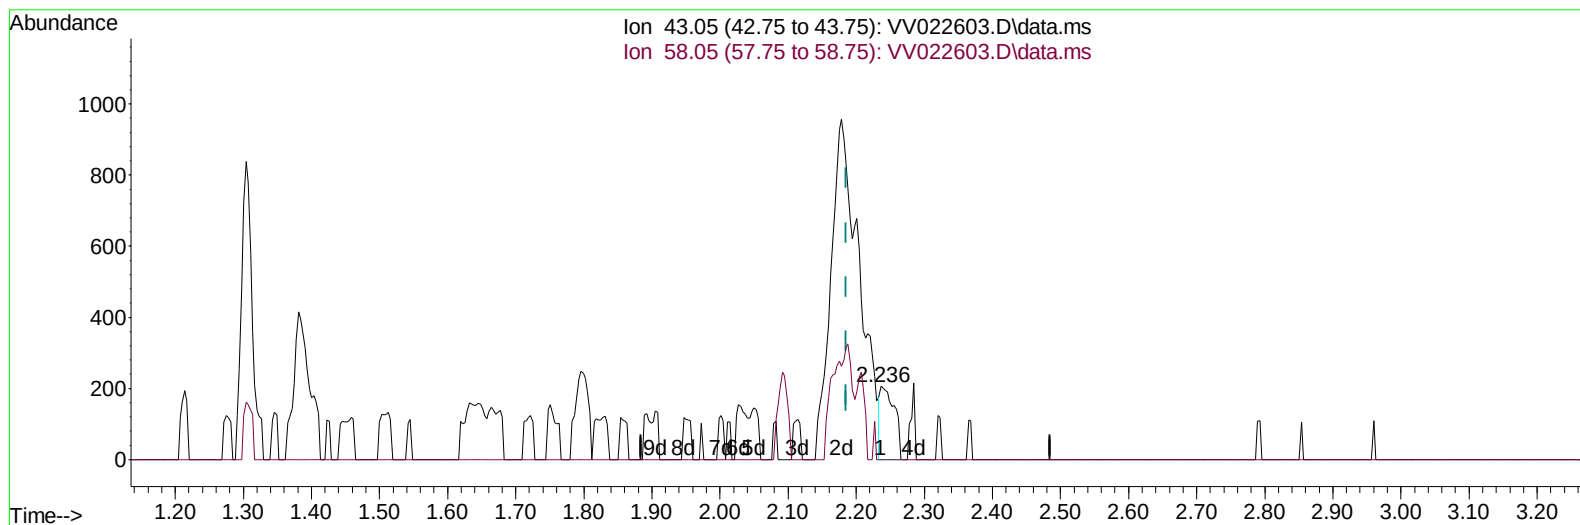

(13) Acetone (T)

2.236min (+ 0.051) 0.27 ug/L

response 292

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	7.19
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022603.D
 Acq On : 06 Oct 2021 05:26
 Operator : SY/MD
 Sample : M4050-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C4

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:43 AM

Quant Time: Oct 06 08:10:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

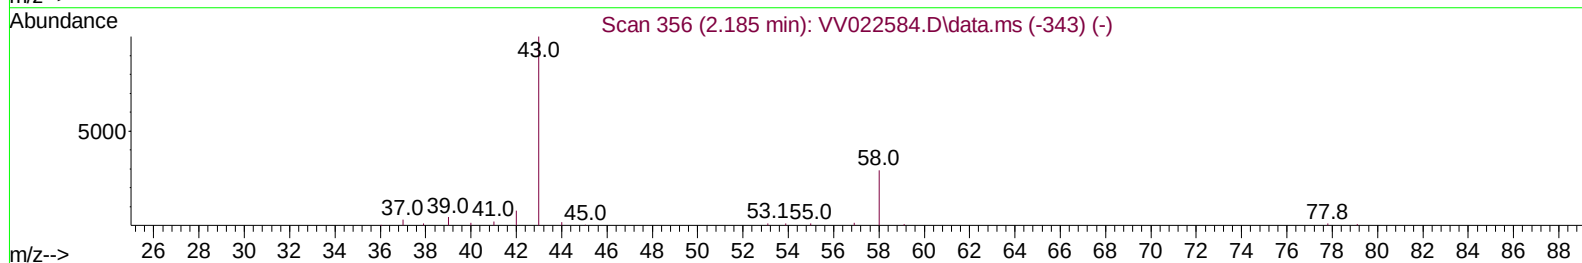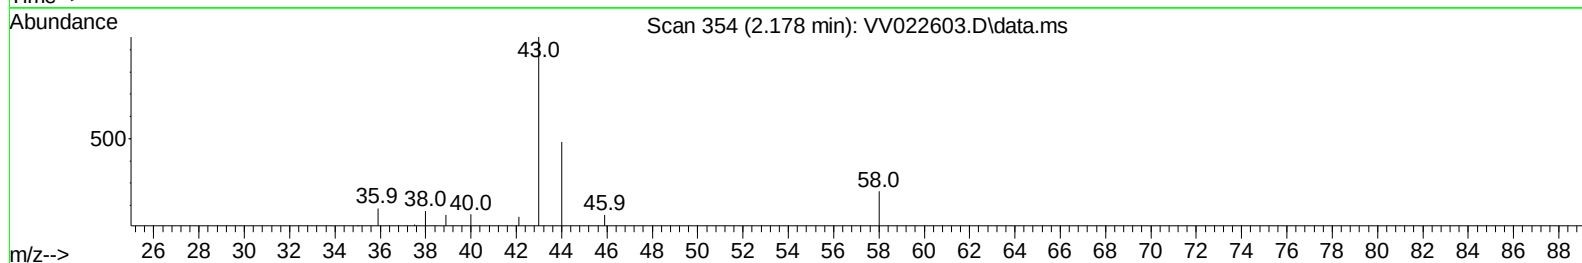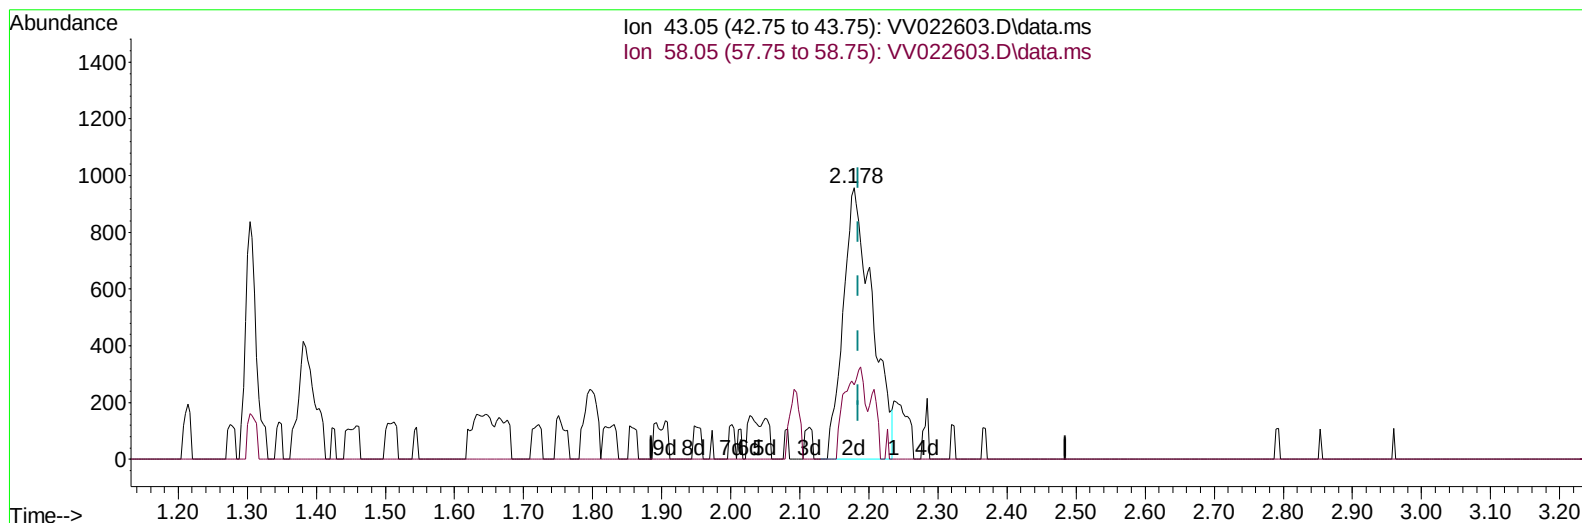

TIC: VV022603.D\data.ms

(13) Acetone (T)

2.178min (-0.007) 2.61 ug/L m

response 2769

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	0.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022603.D
 Acq On : 06 Oct 2021 05:26
 Operator : SY/MD
 Sample : M4050-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C4

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:43 AM

Quant Time: Oct 06 08:10:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	104301	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	103807	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	47893	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	15145	4.532	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	90.600%		
7) Chloroethane-d5	1.564	69	21777	4.834	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	96.600%		
11) 1,1-Dichloroethene-d2	2.105	63	29466	3.039	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	60.800%		
20) 2-Butanone-d5	3.889	46	94738	47.959	ug/L	-0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	95.920%		
24) Chloroform-d	4.349	84	54476	4.233	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.600%		
26) 1,2-Dichloroethane-d4	5.034	65	28554	4.710	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	94.200%		
32) Benzene-d6	5.053	84	98332	4.204	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.000%		
36) 1,2-Dichloropropane-d6	6.072	67	34749	4.210	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	84.200%		
41) Toluene-d8	7.320	98	77166	3.935	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	78.800%		
43) trans-1,3-Dichloroprop...	7.628	79	8288	3.795	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	75.800%		
46) 2-Hexanone-d5	8.091	63	60033	44.392	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	88.780%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27058	4.315	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	86.200%		
66) 1,2-Dichlorobenzene-d4	11.628	152	35649	4.812	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	96.200%		
Target Compounds						
13) Acetone	2.178	43	2769m	2.607	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022603.D
Acq On : 06 Oct 2021 05:26
Operator : SY/MD
Sample : M4050-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C4

Manual Integrations
APPROVED

MMDadoda
10/7/2021 9:33:43 AM

Quant Time: Oct 06 08:10:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 07:50:25 2021
Response via : Initial Calibration

