

(QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022608.D
Acq On : 06 Oct 2021 07:27
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
LabSampleId :
VSTDCCC005EC

Quant Time: Oct 06 08:11:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 07:50:25 2021
Response via : Initial Calibration

Manual Integrations APPROVED

MMDadoda
10/7/2021 9:33:56 AM

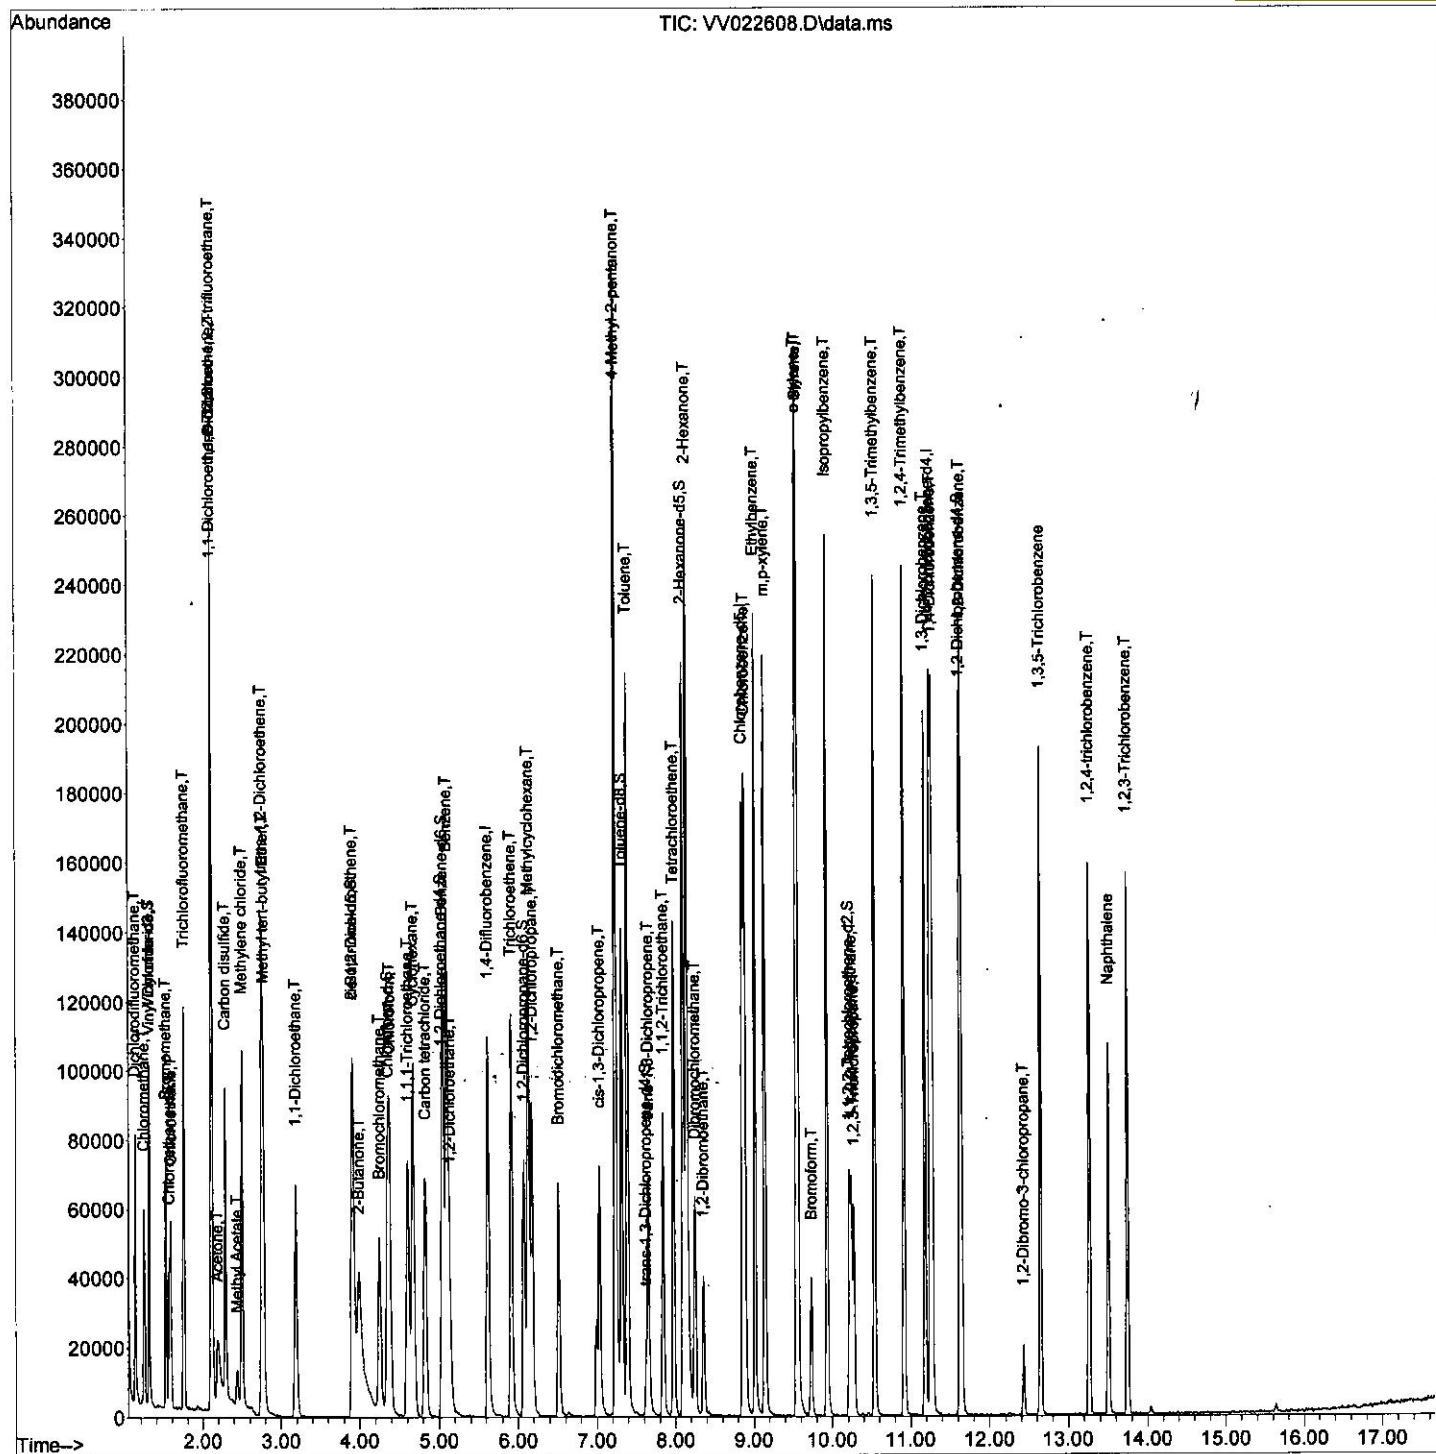

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022608.D
 Acq On : 06 Oct 2021 07:27
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Quant Time: Oct 06 08:11:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:56 AM

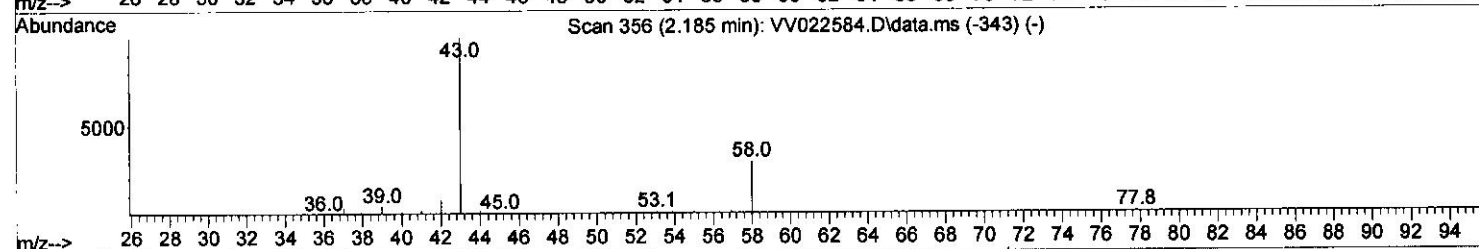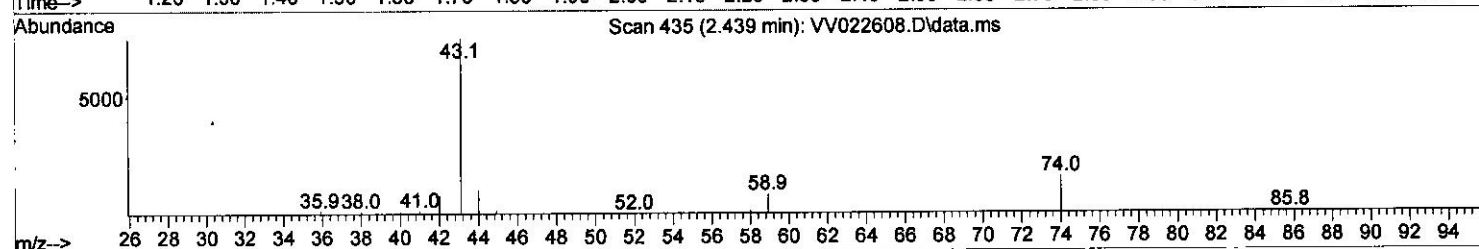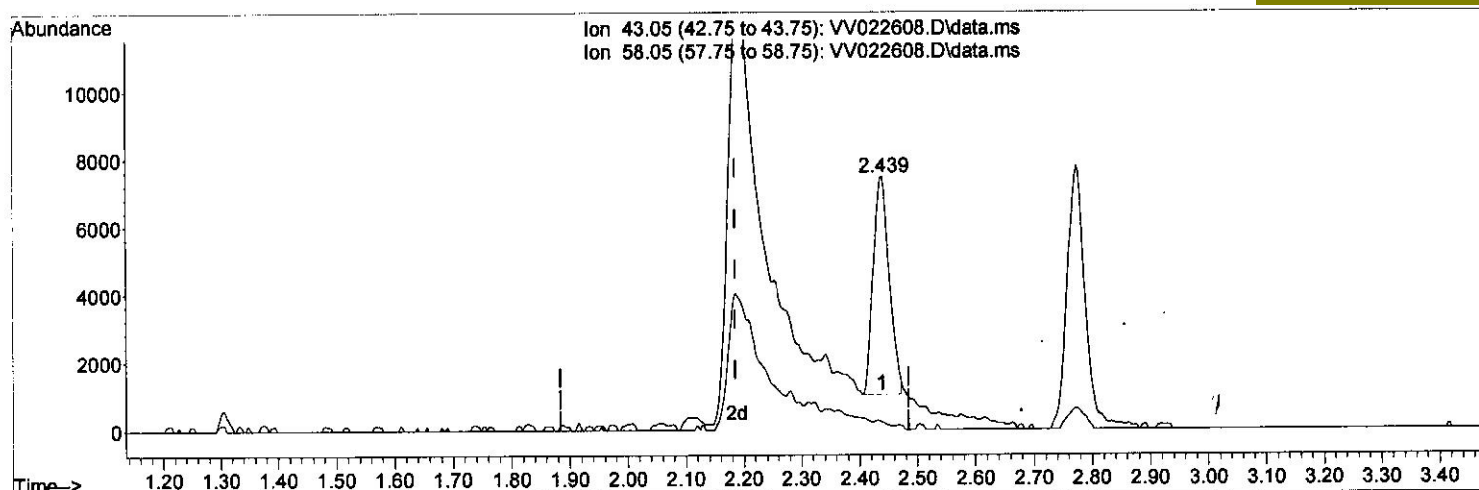

TIC: VV022608.D\data.ms

(13) Acetone (T)

2.439min (+ 0.254) 12.37 ug/L

response 12255

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	7.69
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)





Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022608.D
 Acq On : 06 Oct 2021 07:27
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:56 AM

Quant Time: Oct 06 08:11:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

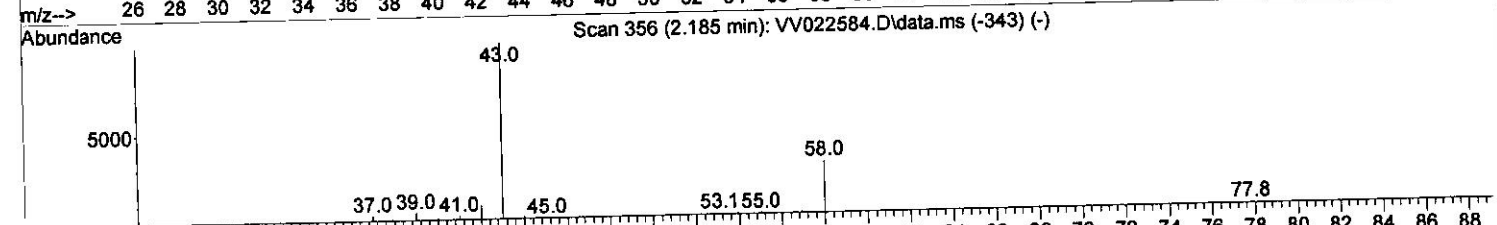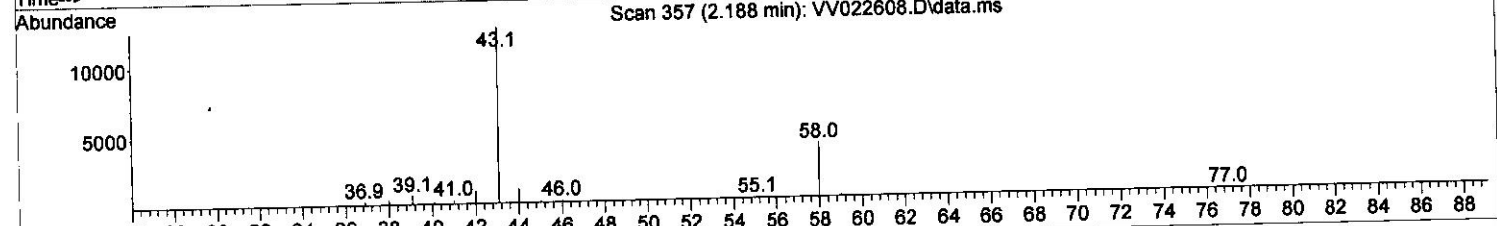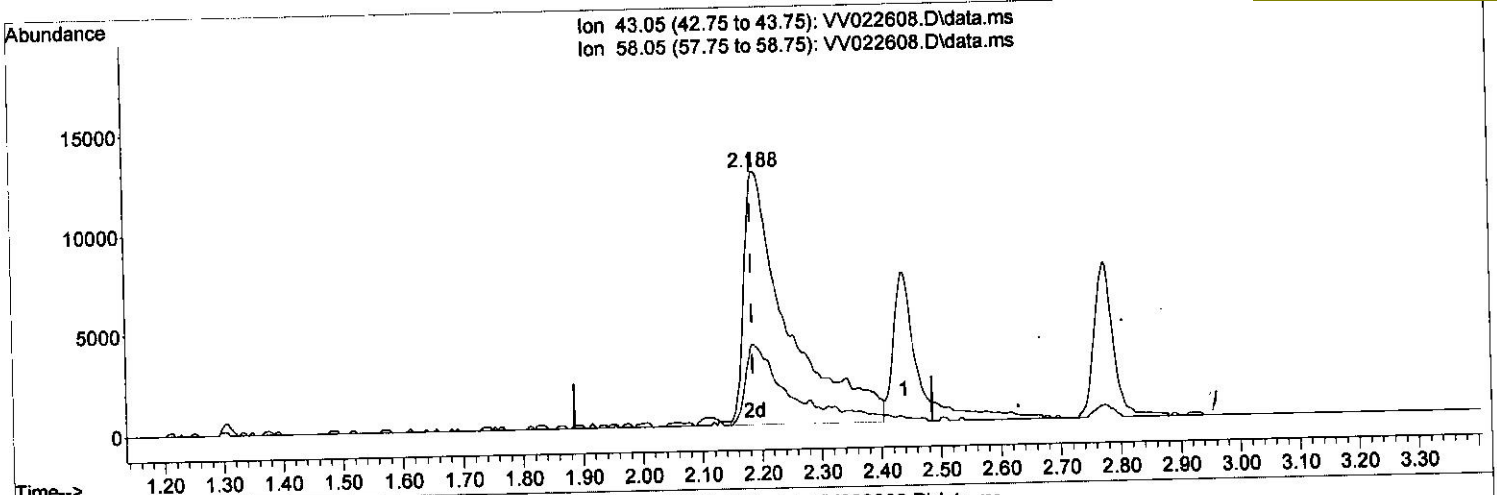

(13) Acetone (T)

2.188min (+ 0.003) 64.97 ug/L m 10/20/21

response 64391

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	8.80	1.46
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100521\
 Data File : VW022608.D
 Acq On : 06 Oct 2021 07:27
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:56 AM

Quant Time: Oct 06 08:11:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	97303	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	96379	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52964	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	16314	5.233	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery = 104.600%			
7) Chloroethane-d5	1.565	69	23208	5.523	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery = 110.400%			
11) 1,1-Dichloroethene-d2	2.108	63	48790	5.394	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery = 107.800%			
20) 2-Butanone-d5	3.908	46	93759	50.877	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery = 101.760%			
24) Chloroform-d	4.352	84	63034	5.251	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery = 105.000%			
26) 1,2-Dichloroethane-d4	5.034	65	31015	5.484	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery = 109.600%			
32) Benzene-d6	5.050	84	108733	5.007	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery = 100.200%			
36) 1,2-Dichloropropane-d6	6.072	67	37402	4.881	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery = 97.600%			
41) Toluene-d8	7.317	98	93390	5.129	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery = 102.600%			
43) trans-1,3-Dichloroprop...	7.625	79	10322	5.090	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery = 101.800%			
46) 2-Hexanone-d5	8.095	63	80351	63.995	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery = 128.000%			
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31903	5.480	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery = 109.600%			
66) 1,2-Dichlorobenzene-d4	11.625	152	41499	5.065	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery = 101.400%			
Target Compounds						
2) Dichlorodifluoromethane	1.127	85	41827	5.644	ug/L	95
3) Chloromethane	1.240	50	43567	5.871	ug/L	98
5) Vinyl chloride	1.307	62	44637	5.960	ug/L	98
6) Bromomethane	1.520	94	28879	5.809	ug/L	96
8) Chloroethane	1.584	64	28129	5.906	ug/L	96
9) Trichlorofluoromethane	1.751	101	65396	5.837	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	2.114	101	36743	5.703	ug/L	99
12) 1,1-Dichloroethene	2.114	96	34893	5.854	ug/L	93
13) Acetone	2.188	43	64391m	64.974	ug/L	
14) Carbon disulfide	2.288	76	98531	5.651	ug/L	98
15) Methyl Acetate	2.439	43	15548	5.327	ug/L #	81
16) Methylene chloride	2.500	84	41199	5.999	ug/L	98
17) Methyl tert-butyl Ether	2.773	73	88569	5.847	ug/L	98
18) trans-1,2-Dichloroethene	2.754	96	40054	6.166	ug/L	96
19) 1,1-Dichloroethane	3.185	63	67104	5.758	ug/L	99
21) 2-Butanone	3.992	43	77812	49.047	ug/L	98
22) cis-1,2-Dichloroethene	3.908	96	39002	5.534	ug/L	92
23) Bromochloromethane	4.246	128	19130	5.766	ug/L	95

MD
 10/20/21

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100521\
 Data File : VW022608.D
 Acq On : 06 Oct 2021 07:27
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTDCCC005EC

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:56 AM

Quant Time: Oct 06 08:11:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
25) Chloroform	4.375	83	72318	5.682	ug/L	99
27) 1,2-Dichloroethane	5.133	62	40289	5.948	ug/L #	94
29) 1,1,1-Trichloroethane	4.606	97	60257	5.472	ug/L	98
30) Cyclohexane	4.670	56	52233	5.235	ug/L	98
31) Carbon tetrachloride	4.825	117	53494	5.476	ug/L	98
33) Benzene	5.098	78	146381	5.636	ug/L	100
34) Trichloroethene	5.915	95	38712	5.129	ug/L	98
35) Methylcyclohexane	6.130	83	52451	4.959	ug/L	97
37) 1,2-Dichloropropane	6.175	63	35584	5.612	ug/L	100
38) Bromodichloromethane	6.513	83	45128	5.616	ug/L	95
39) cis-1,3-Dichloropropene	7.031	75	44750	5.236	ug/L	98
40) 4-Methyl-2-pentanone	7.233	43	232522	66.619	ug/L	99
42) Toluene	7.387	91	157769	5.782	ug/L	99
44) trans-1,3-Dichloropropene	7.654	75	39508	5.538	ug/L	97
45) 1,1,2-Trichloroethane	7.841	97	27344	5.777	ug/L	94
47) Tetrachloroethene	7.979	164	32813	5.590	ug/L	94
48) 2-Hexanone	8.143	43	171021	68.108	ug/L	100
49) Dibromochloromethane	8.249	129	33435	5.993	ug/L	99
50) 1,2-Dibromoethane	8.355	107	26881	6.109	ug/L #	94
51) Chlorobenzene	8.883	112	101131	5.663	ug/L	98
52) Ethylbenzene	9.014	91	157177	5.613	ug/L	98
53) m,p-xylene	9.140	106	62864	5.888	ug/L	97
54) o-xylene	9.545	106	62289	5.865	ug/L	97
55) Styrene	9.561	104	106977	5.924	ug/L	96
57) 1,1,1,2-Tetrachloroethane	10.243	83	30272	5.894	ug/L	98
59) Bromoform	9.735	173	18502	5.955	ug/L	98
60) Isopropylbenzene	9.934	105	161982	5.688	ug/L	100
61) 1,2,3-Trichloropropane	10.275	75	23536	5.995	ug/L	97
62) 1,3,5-Trimethylbenzene	10.542	105	129789	5.622	ug/L	100
63) 1,2,4-Trimethylbenzene	10.915	105	133339	5.685	ug/L	99
64) 1,3-Dichlorobenzene	11.181	146	84174	5.774	ug/L	99
65) 1,4-Dichlorobenzene	11.275	146	84304	5.654	ug/L	97
67) 1,2-Dichlorobenzene	11.645	146	81012	5.965	ug/L	97
68) 1,2-Dibromo-3-chloropr...	12.429	75	4503	6.001	ug/L	93
69) 1,3,5-Trichlorobenzene	12.648	180	59888	5.488	ug/L	99
70) 1,2,4-trichlorobenzene	13.262	180	49556	5.658	ug/L	98
71) Naphthalene	13.503	128	84998	5.923	ug/L	99
72) 1,2,3-Trichlorobenzene	13.744	180	47941	5.957	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed