

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022561.D
 Acq On : 05 Oct 2021 10:38
 Operator : SY/MD
 Sample : VV1005WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Quant Time: Oct 06 06:32:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 05:22:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	99543	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	97463	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	44301	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	18997	5.956	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	119.200%	
7) Chloroethane-d5	1.565	69	26267	6.110	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	122.200%	
11) 1,1-Dichloroethene-d2	2.105	63	36401	3.934	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.600%	
20) 2-Butanone-d5	3.905	46	74802	39.677	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	79.360%	
24) Chloroform-d	4.349	84	60924	4.961	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
26) 1,2-Dichloroethane-d4	5.034	65	31046	5.366	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.400%	
32) Benzene-d6	5.050	84	114694	5.222	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.400%	
36) 1,2-Dichloropropane-d6	6.072	67	37226	4.804	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.000%	
41) Toluene-d8	7.317	98	92449	5.021	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.400%	
43) trans-1,3-Dichloroprop...	7.629	79	8965	4.372	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.400%	
46) 2-Hexanone-d5	8.092	63	59769	47.073	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.140%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27651	4.697	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	39407	5.751	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.000%	
Target Compounds						Qvalue
34) Trichloroethene	5.925	95	931	0.122	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022561.D
Acq On : 05 Oct 2021 10:38
Operator : SY/MD
Sample : VV1005WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Time: Oct 06 06:32:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 05:22:36 2021
Response via : Initial Calibration

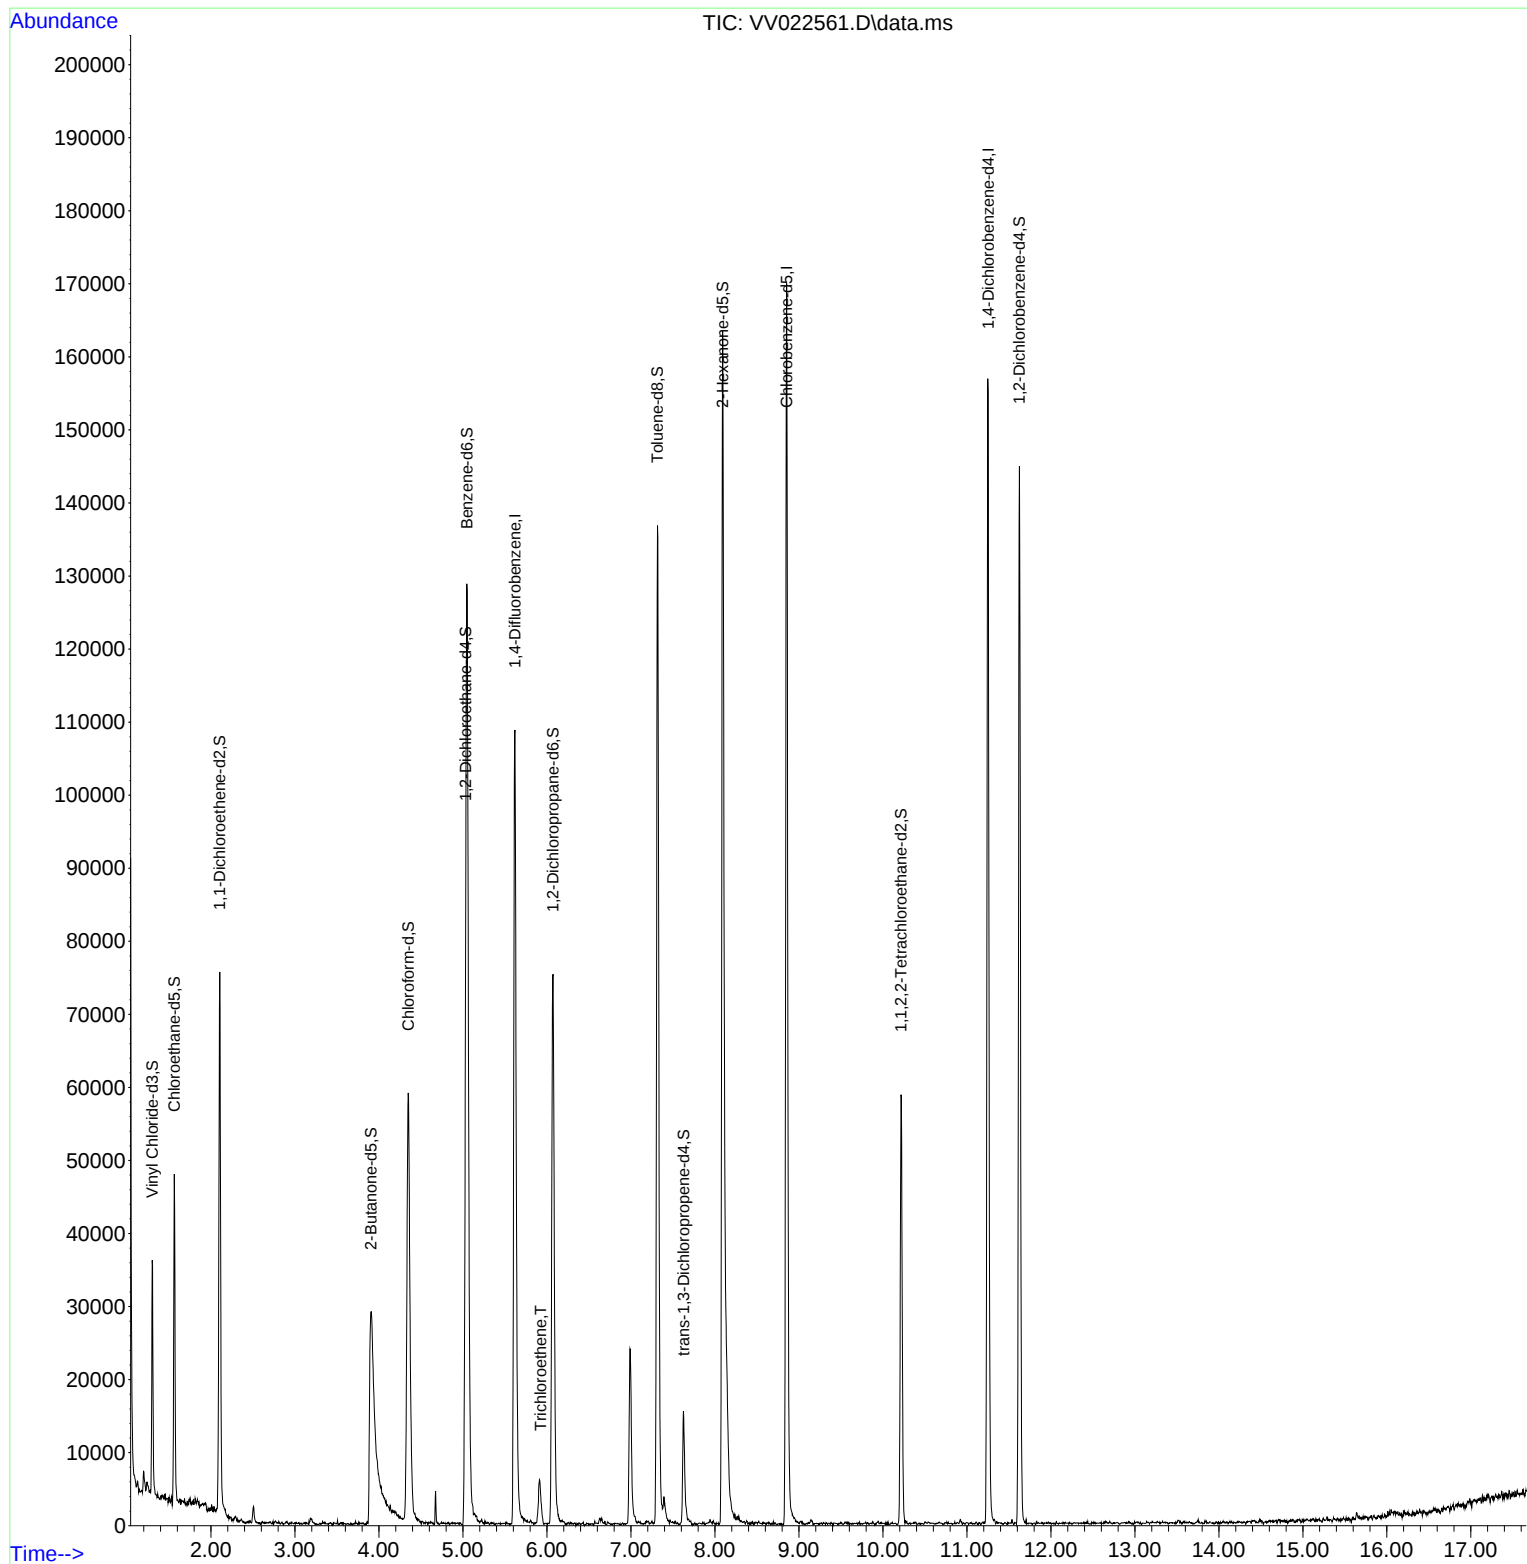

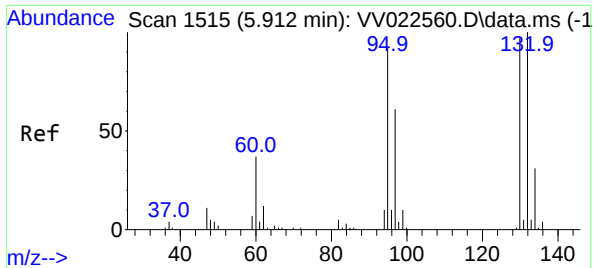

#34
 Trichloroethene
 Concen: 0.122 ug/L
 RT: 5.925 min Scan# 1519
 Delta R.T. 0.013 min
 Lab File: VV022561.D
 Acq: 05 Oct 2021 10:38

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Tgt Ion: 95 Resp: 931

Ion	Ratio	Lower	Upper
95	100		
97	59.5	46.5	86.5
132	104.2	73.0	135.6
130	105.4	76.1	141.3

