

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022597.D
 Acq On : 06 Oct 2021 03:01
 Operator : SY/MD
 Sample : M4050-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7B8

Quant Time: Oct 06 08:08:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	106193	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	105249	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49016	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	15639	4.596	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.000%
7) Chloroethane-d5	1.564	69	22473	4.900	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.000%
11) 1,1-Dichloroethene-d2	2.104	63	30804	3.120	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.400%
20) 2-Butanone-d5	3.883	46	94058	46.766	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.540%
24) Chloroform-d	4.352	84	54615	4.168	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.400%
26) 1,2-Dichloroethane-d4	5.034	65	28742	4.657	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.050	84	100903	4.254	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.000%
36) 1,2-Dichloropropane-d6	6.072	67	34780	4.156	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.200%
41) Toluene-d8	7.320	98	77287	3.887	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.800%
43) trans-1,3-Dichloroprop...	7.628	79	8859	4.001	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.088	63	61561	44.898	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.800%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27190	4.277	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	35928	4.739	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.800%
Target Compounds						
					Qvalue	
13) Acetone	2.172	43	4175	3.860	ug/L	# 40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022597.D
Acq On : 06 Oct 2021 03:01
Operator : SY/MD
Sample : M4050-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B8


Quant Time: Oct 06 08:08:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 07:50:25 2021
Response via : Initial Calibration

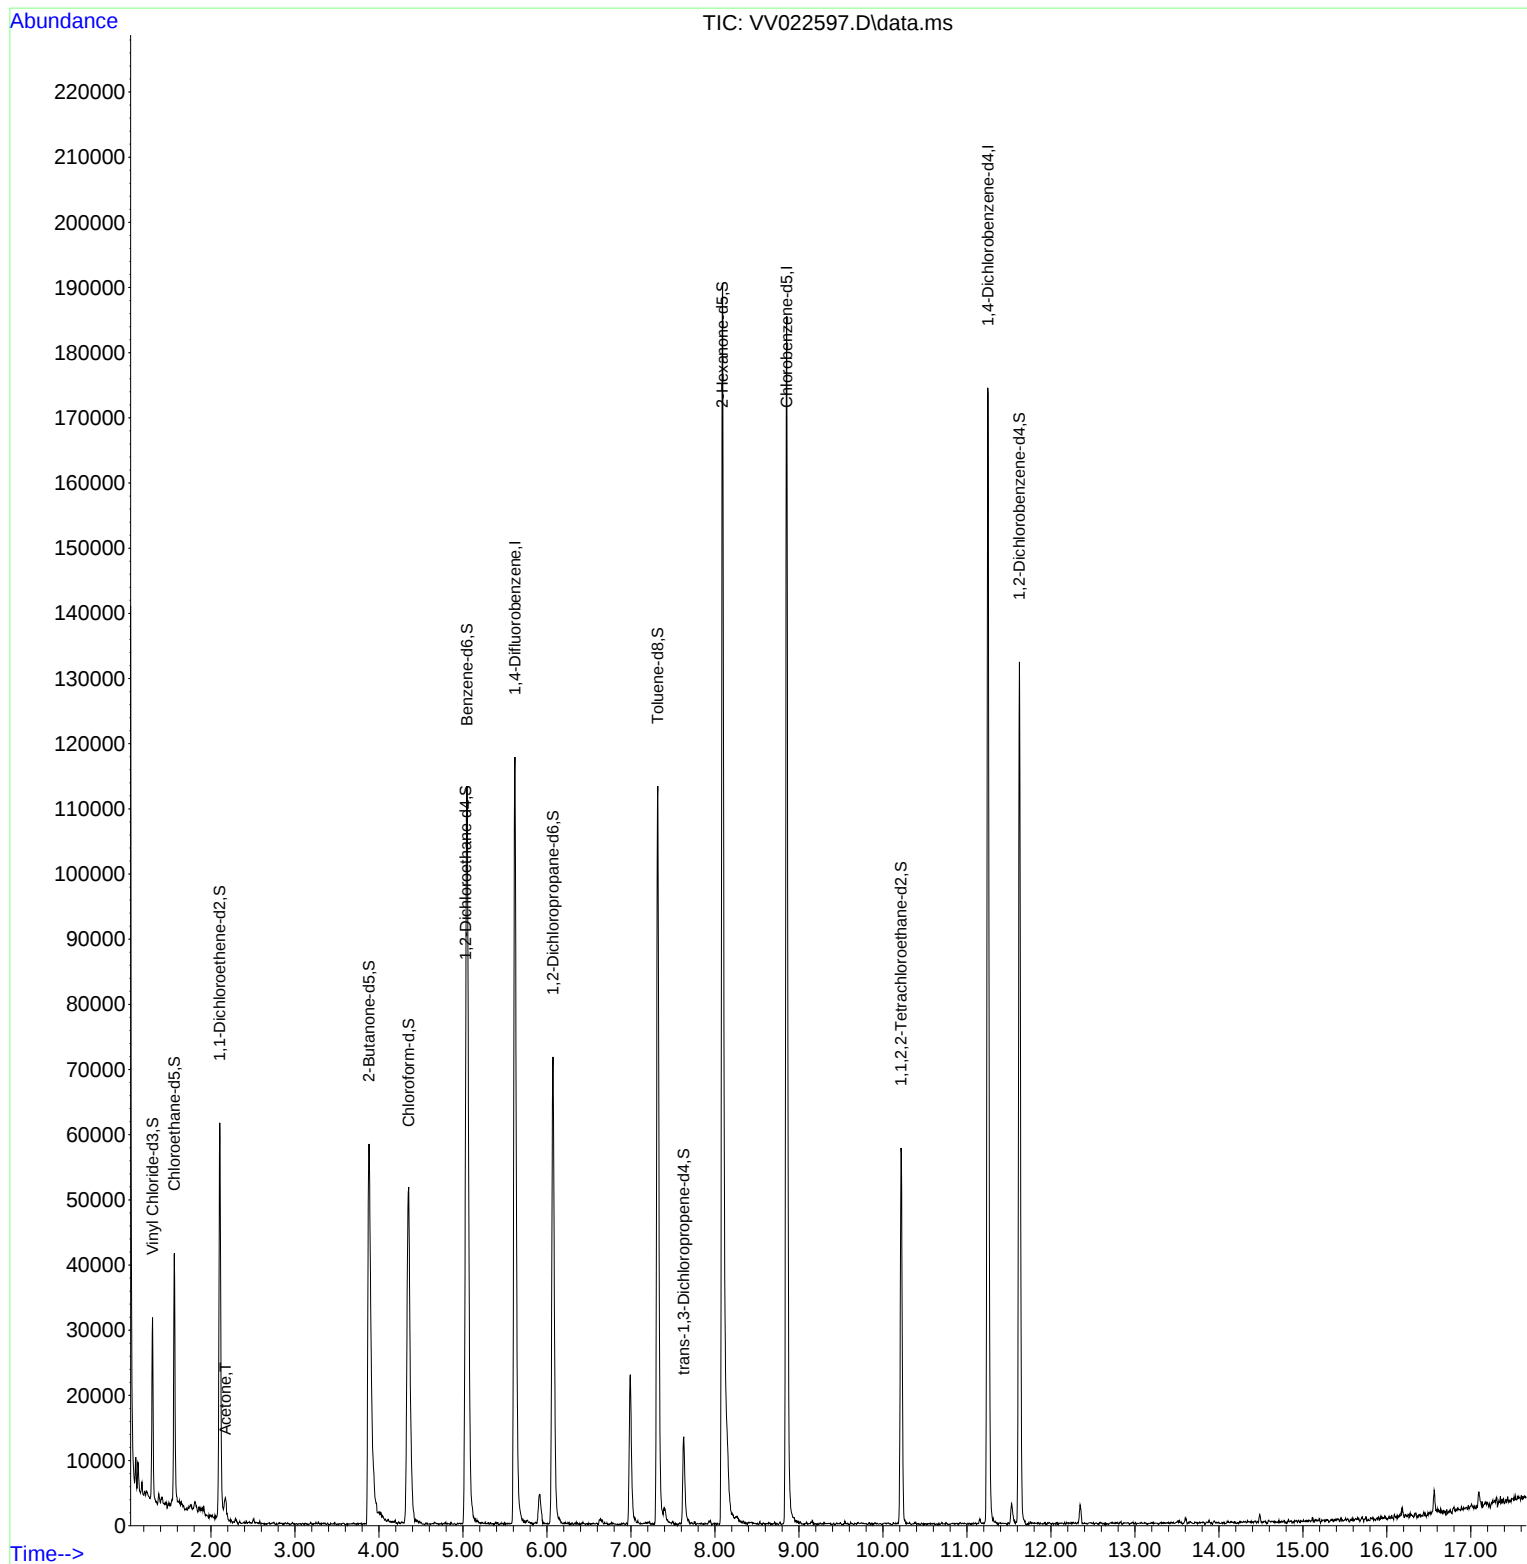

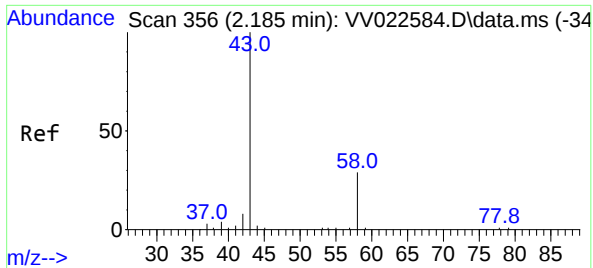

#13
 Acetone
 Concen: 3.860 ug/L
 RT: 2.172 min Scan# 352
 Delta R.T. -0.013 min
 Lab File: VV022597.D
 Acq: 06 Oct 2021 03:01

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7B8

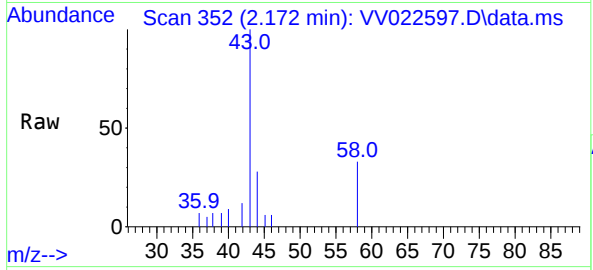

Tgt Ion: 43 Resp: 4175

Ion	Ratio	Lower	Upper
43	100		
58	30.5	0.0	17.6#

