

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100521\
 Data File : VW022602.D
 Acq On : 06 Oct 2021 05:02
 Operator : SY/MD
 Sample : M4050-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C3

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:40 AM

Quant Time: Oct 06 08:09:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	101027	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	98471	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	45243	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	15830	4.891	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	97.800%	
7) Chloroethane-d5	1.565	69	25350	5.810	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	116.200%	
11) 1,1-Dichloroethene-d2	2.105	63	32113	3.419	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.400%	
20) 2-Butanone-d5	3.905	46	95933	50.138	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.280%	
24) Chloroform-d	4.349	84	58276	4.675	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.600%	
26) 1,2-Dichloroethane-d4	5.034	65	31467	5.359	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.200%	
32) Benzene-d6	5.050	84	106216	4.787	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.072	67	36123	4.614	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.200%	
41) Toluene-d8	7.320	98	82983	4.461	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.200%	
43) trans-1,3-Dichloroprop...	7.629	79	8893	4.292	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.800%	
46) 2-Hexanone-d5	8.092	63	68729	53.576	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	107.160%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29564	4.970	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	38891	5.557	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.200%	
Target Compounds					Qvalue	
13) Acetone	2.201	43	3172m	3.083	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022602.D
Acq On : 06 Oct 2021 05:02
Operator : SY/MD
Sample : M4050-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
GB7C3

Manual Integrations
APPROVED

MMDadoda
10/7/2021 9:33:40 AM


Quant Time: Oct 06 08:09:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 07:50:25 2021
Response via : Initial Calibration

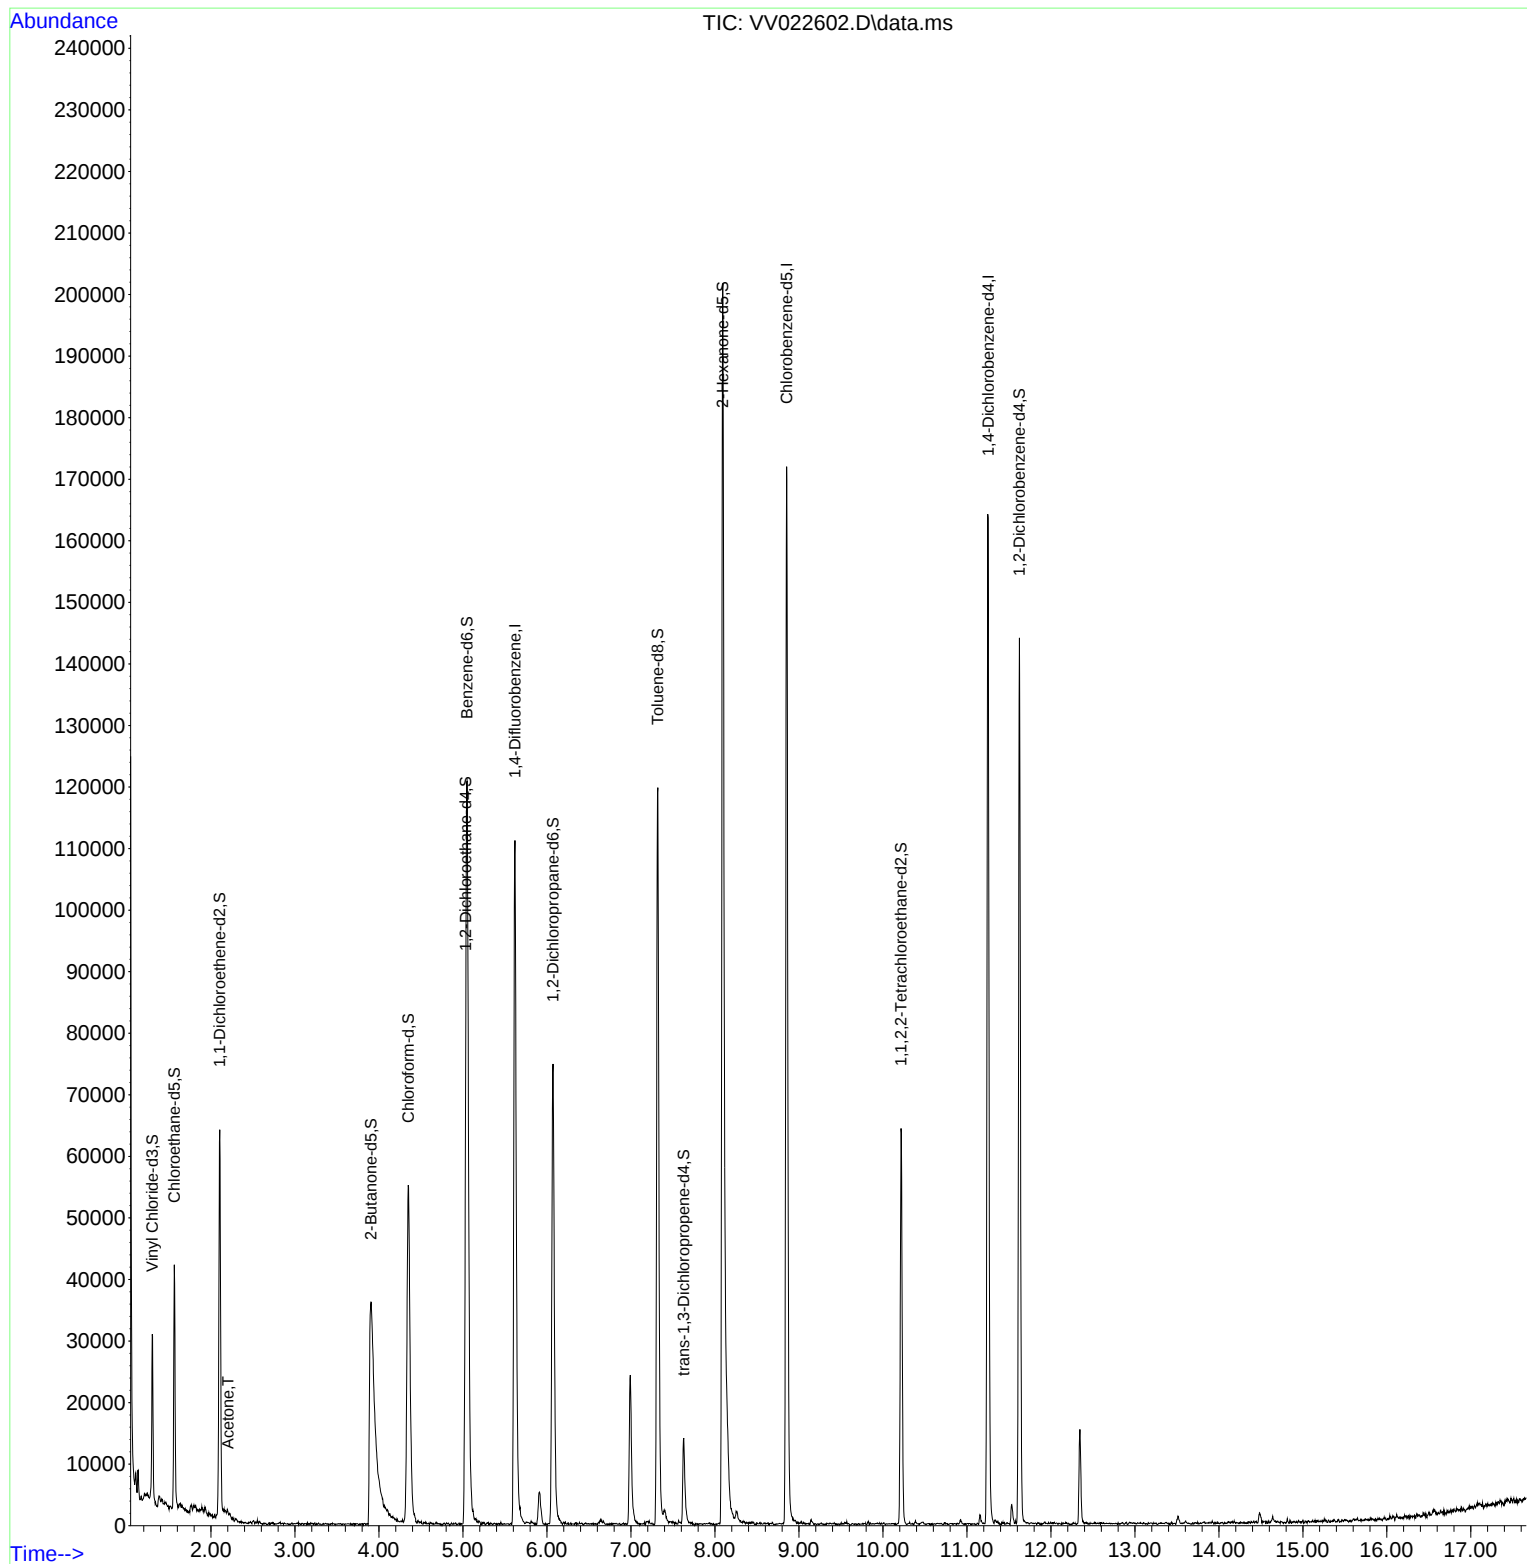

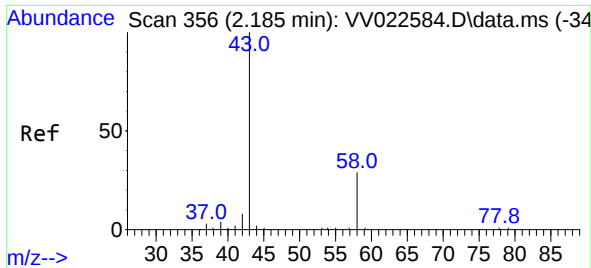

#13
Acetone
Concen: 3.083 ug/L m
RT: 2.201 min Scan# 361
Delta R.T. 0.016 min
Lab File: VV022602.D
Acq: 06 Oct 2021 05:02

Instrument :
MSVOA_V
ClientSampleId :
GB7C3

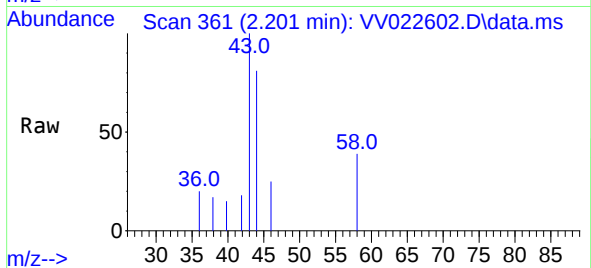

Tgt Ion: 43 Resp: 3172
Ion Ratio Lower Upper
43 100
58 15.4 0.0 17.6

Manual Integrations
APPROVED

MMDadoda
10/7/2021 9:33:40 AM

