

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100521\
 Data File : VW022603.D
 Acq On : 06 Oct 2021 05:26
 Operator : SY/MD
 Sample : M4050-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C4

Manual Integrations
 APPROVED

MMDadoda
 10/7/2021 9:33:43 AM

Quant Time: Oct 06 08:10:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 06 07:50:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	104301	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	103807	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	47893	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	15145	4.532	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.600%
7) Chloroethane-d5	1.564	69	21777	4.834	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.600%
11) 1,1-Dichloroethene-d2	2.105	63	29466	3.039	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.800%
20) 2-Butanone-d5	3.889	46	94738	47.959	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.920%
24) Chloroform-d	4.349	84	54476	4.233	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	5.034	65	28554	4.710	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	5.053	84	98332	4.204	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	6.072	67	34749	4.210	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.200%
41) Toluene-d8	7.320	98	77166	3.935	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.800%
43) trans-1,3-Dichloroprop...	7.628	79	8288	3.795	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.800%
46) 2-Hexanone-d5	8.091	63	60033	44.392	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.780%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27058	4.315	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.200%
66) 1,2-Dichlorobenzene-d4	11.628	152	35649	4.812	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds					Qvalue	
13) Acetone	2.178	43	2769m	2.607	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022603.D
Acq On : 06 Oct 2021 05:26
Operator : SY/MD
Sample : M4050-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
GB7C4

Manual Integrations
APPROVED

MMDadoda
10/7/2021 9:33:43 AM

Quant Time: Oct 06 08:10:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 06 07:50:25 2021
Response via : Initial Calibration

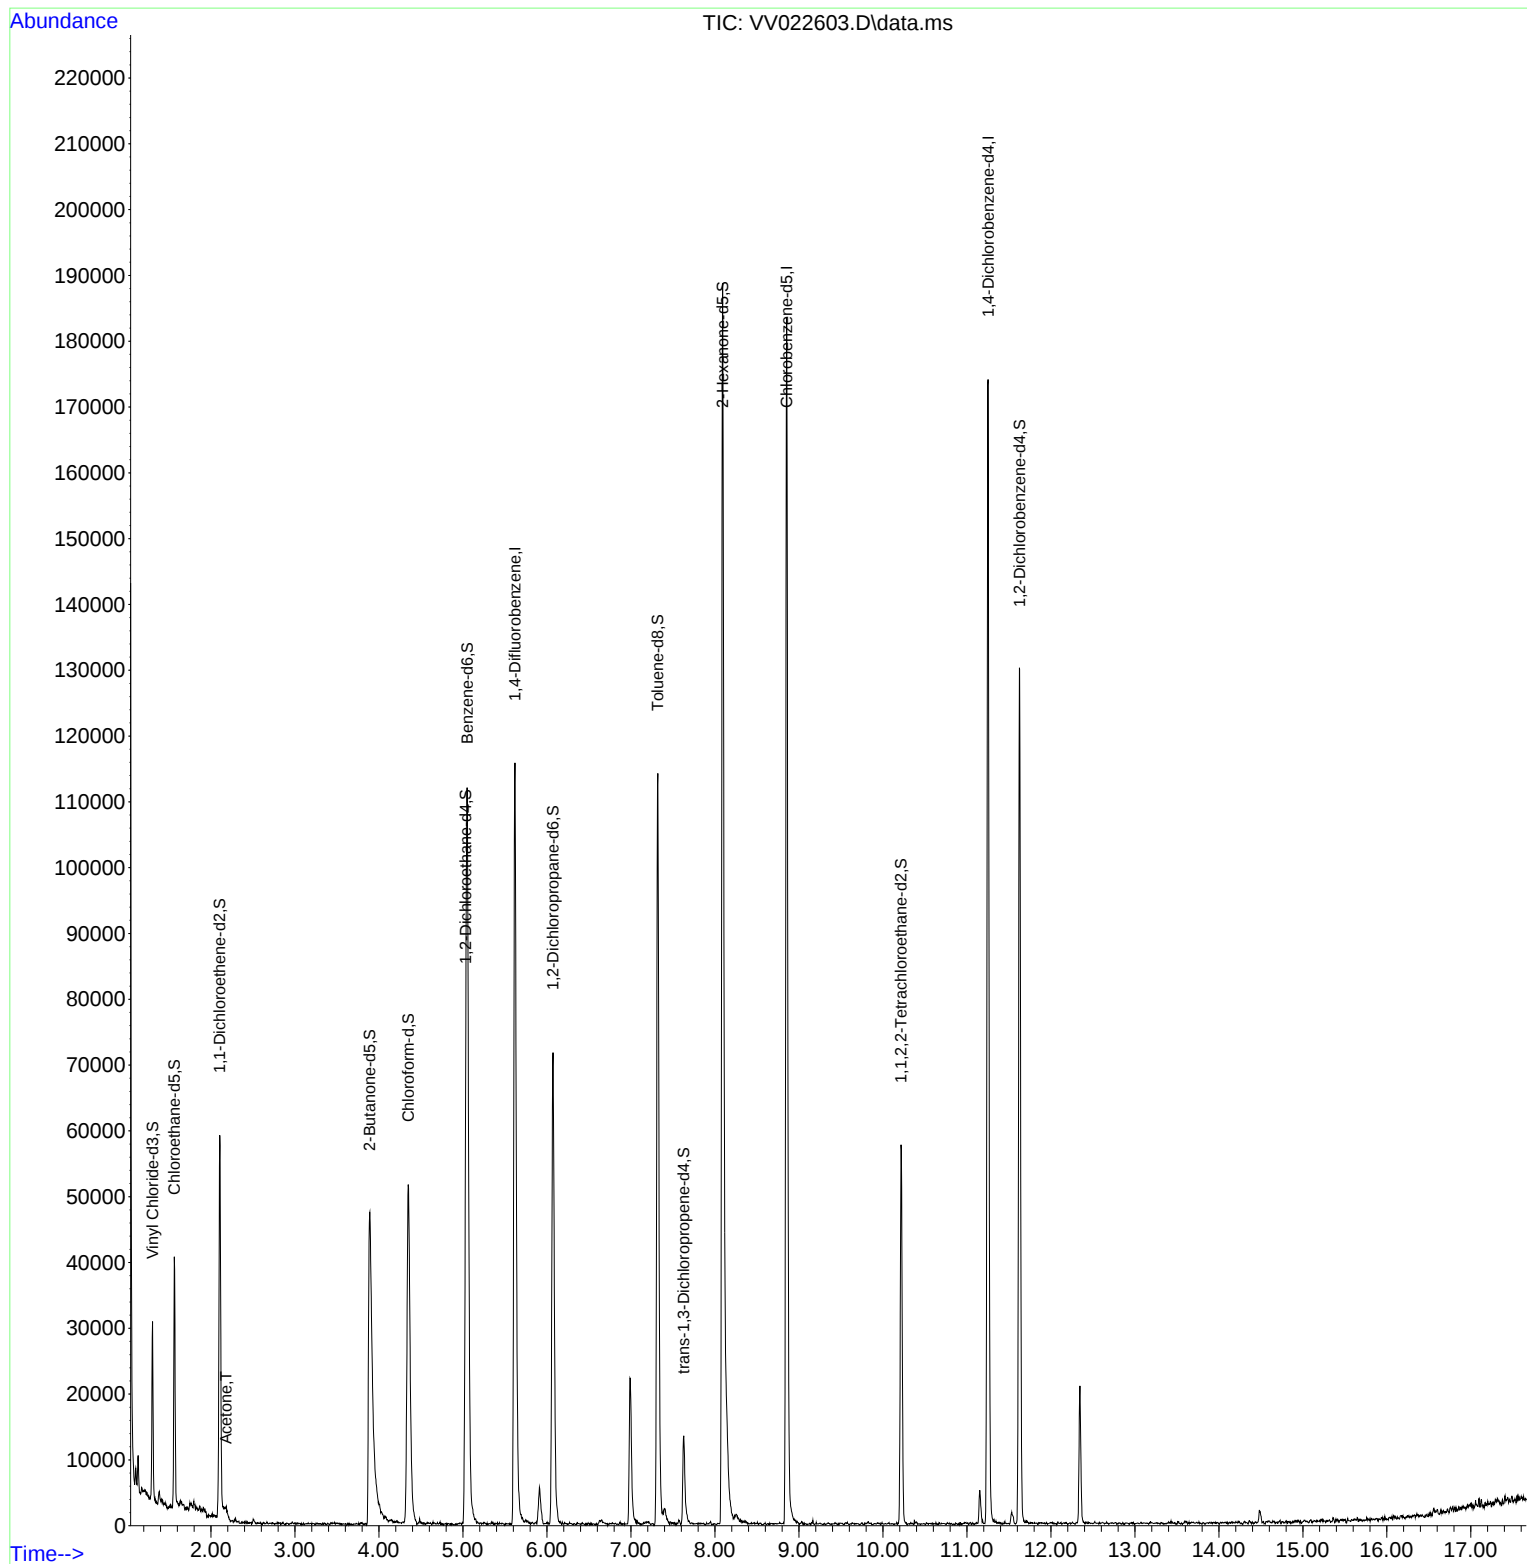

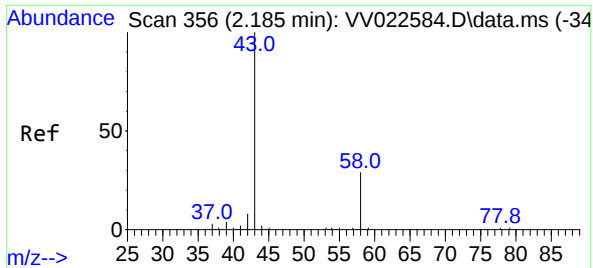

#13
Acetone
Concen: 2.607 ug/L m
RT: 2.178 min Scan# 354
Delta R.T. -0.007 min
Lab File: VV022603.D
Acq: 06 Oct 2021 05:26

Tgt Ion: 43 Resp: 2769
Ion Ratio Lower Upper
43 100
58 0.8 0.0 17.6

Instrument :
MSVOA_V
ClientSampleId :
GB7C4

Manual Integrations
APPROVED

MMDadoda
10/7/2021 9:33:43 AM

