

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022562.D
 Acq On : 05 Oct 2021 11:02
 Operator : SY/MD
 Sample : M3967-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0T6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	91	rVV	29506	28729	8.12%	1.069%
2	1.564	155	163	174	rBV	40149	45884	12.97%	1.708%
3	2.105	321	331	347	rVB	63570	91655	25.91%	3.411%
4	3.902	878	890	917	rBV2	30360	116686	32.99%	4.342%
5	4.349	1013	1029	1052	rBV	67358	178165	50.37%	6.630%
6	5.047	1231	1246	1276	rBV2	124860	309026	87.37%	11.500%
7	5.619	1410	1424	1450	rBV	114440	234736	66.36%	8.735%
8	5.911	1503	1515	1529	rVB5	9031	19703	5.57%	0.733%
9	6.072	1552	1565	1591	rBV2	74559	155298	43.91%	5.779%
10	6.989	1840	1850	1871	rBV3	24933	46779	13.23%	1.741%
11	7.317	1940	1952	1972	rBV	127639	227510	64.32%	8.466%
12	7.390	1972	1975	1988	rVB6	2535	4689	1.33%	0.174%
13	7.625	2038	2048	2067	rBV2	14290	26367	7.45%	0.981%
14	8.095	2183	2194	2239	rBV3	148159	353710	100.00%	13.163%
15	8.853	2419	2430	2446	rBV	173459	282863	79.97%	10.526%
16	10.220	2843	2855	2872	rVB	52599	83740	23.67%	3.116%
17	11.249	3165	3175	3193	rBV	162733	256061	72.39%	9.529%
18	11.538	3253	3265	3277	rBV4	2532	4701	1.33%	0.175%
19	11.625	3280	3292	3310	rBV	138681	220900	62.45%	8.220%




Sum of corrected areas: 2687202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022562.D
Acq On : 05 Oct 2021 11:02
Operator : SY/MD
Sample : M3967-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

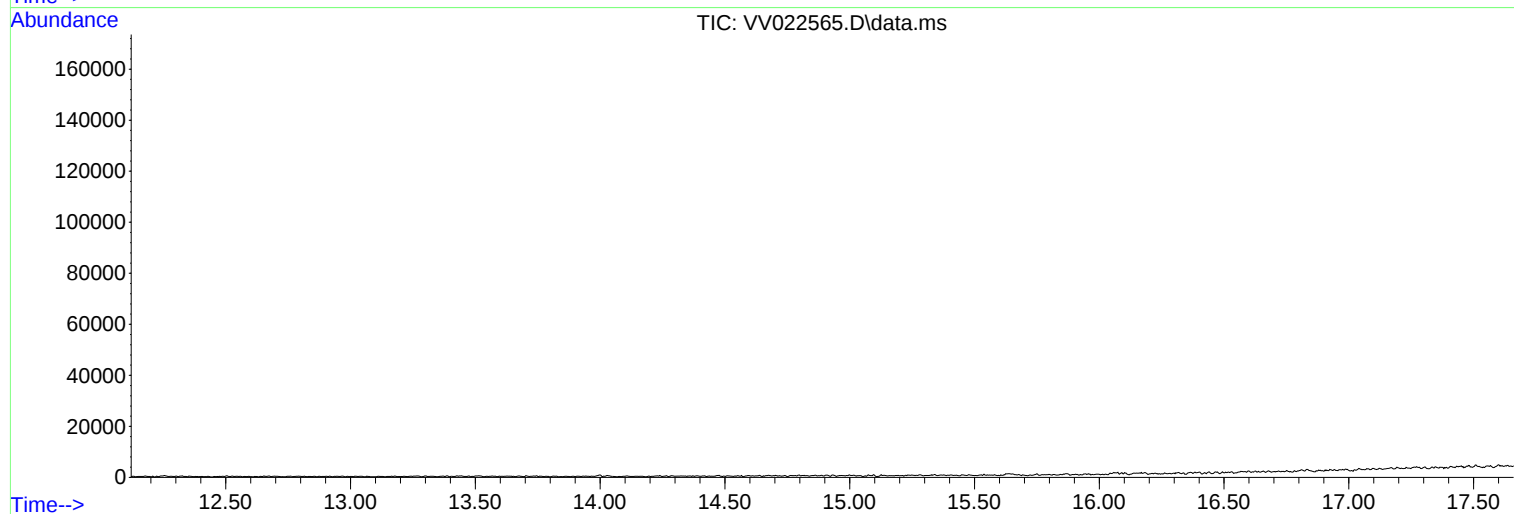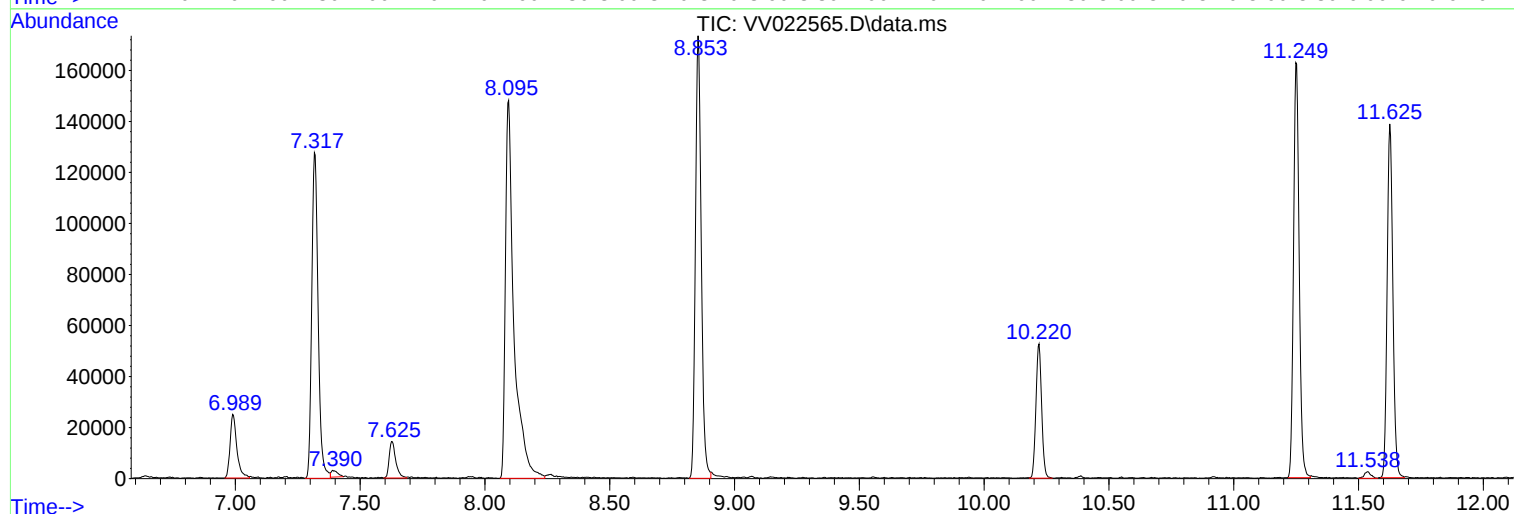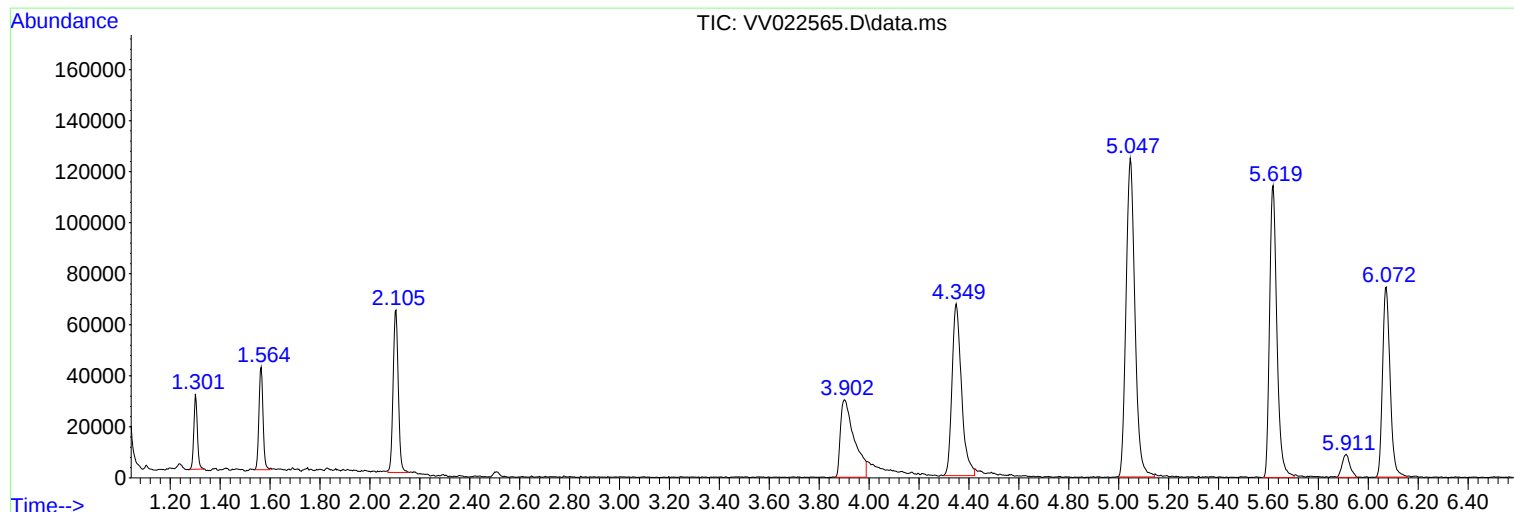

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022562.D
Acq On : 05 Oct 2021 11:02
Operator : SY/MD
Sample : M3967-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022562.D
Acq On : 05 Oct 2021 11:02
Operator : SY/MD
Sample : M3967-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
