

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022563.D
 Acq On : 05 Oct 2021 11:25
 Operator : SY/MD
 Sample : M3967-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0S8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.237	58	61	71	rVB6	2552	3794	1.14%	0.144%
2	1.301	72	81	88	rBV	28538	28992	8.72%	1.098%
3	1.565	153	163	174	rBV	37900	45221	13.60%	1.712%
4	1.941	273	280	288	rVB8	3792	6471	1.95%	0.245%
5	2.102	320	330	348	rVB4	73317	118944	35.77%	4.503%
6	2.777	529	540	559	rVB2	11857	27733	8.34%	1.050%
7	3.912	881	893	918	rBV2	39926	135346	40.70%	5.124%
8	4.349	1010	1029	1057	rVB2	53836	140702	42.31%	5.327%
9	5.043	1230	1245	1269	rBV2	121870	292527	87.96%	11.074%
10	5.619	1411	1424	1446	rBV	111165	225711	67.87%	8.545%
11	5.915	1505	1516	1532	rBV10	8115	18859	5.67%	0.714%
12	6.072	1552	1565	1587	rBV	69136	144326	43.40%	5.464%
13	6.992	1839	1851	1875	rBV	23683	43923	13.21%	1.663%
14	7.317	1938	1952	1970	rBV	119279	209227	62.91%	7.921%
15	7.629	2040	2049	2067	rBV2	13304	24402	7.34%	0.924%
16	7.979	2148	2158	2170	rVB3	14016	24014	7.22%	0.909%
17	8.095	2184	2194	2232	rBV2	152519	332565	100.00%	12.590%
18	8.854	2419	2430	2455	rBV	166623	276619	83.18%	10.472%
19	10.220	2844	2855	2874	rBV2	54485	87466	26.30%	3.311%
20	11.249	3165	3175	3191	rBV	154869	244062	73.39%	9.240%
21	11.538	3256	3265	3277	rVB4	2776	4922	1.48%	0.186%
22	11.625	3282	3292	3308	rBV	130309	205658	61.84%	7.786%


Sum of corrected areas: 2641484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022563.D
Acq On : 05 Oct 2021 11:25
Operator : SY/MD
Sample : M3967-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0S8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

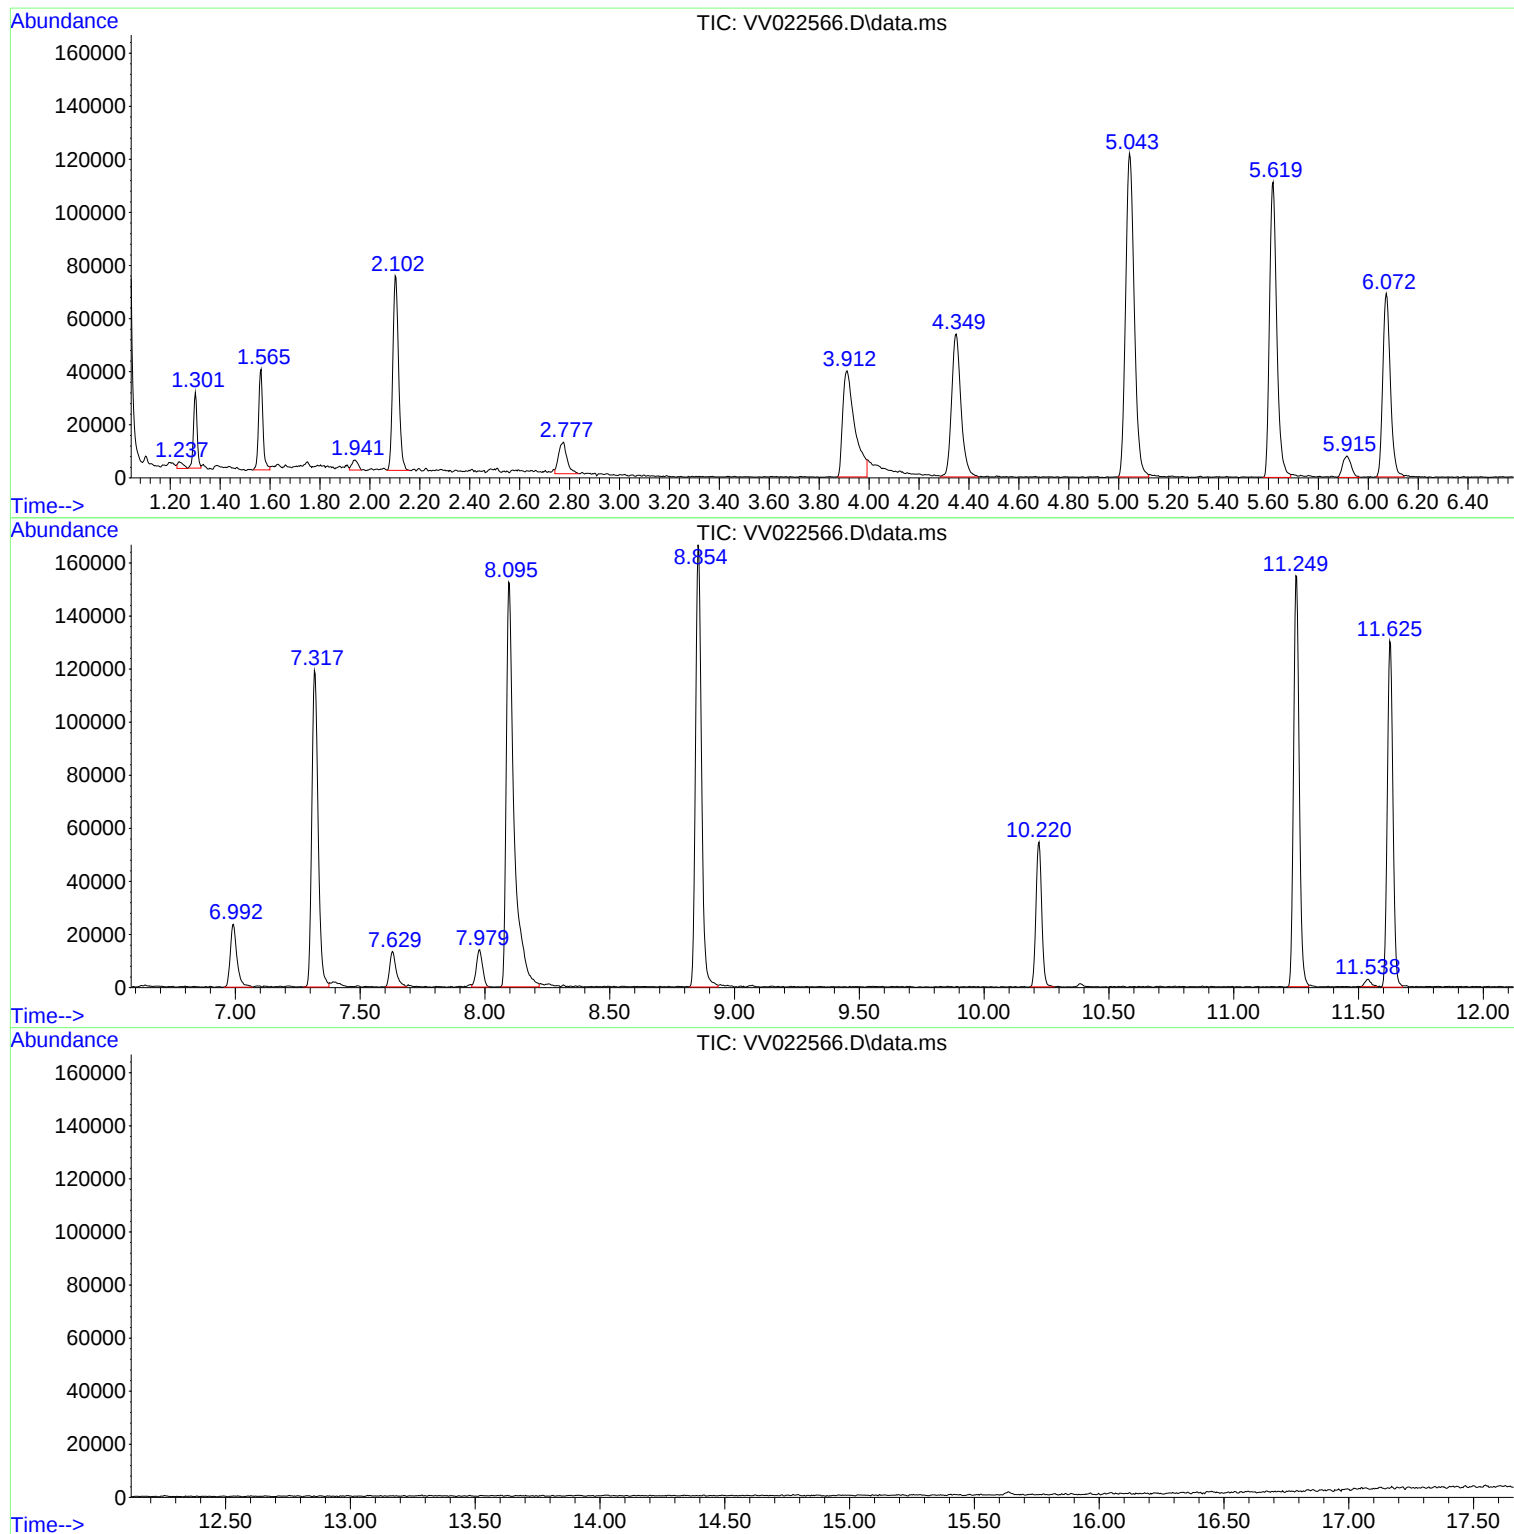

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022563.D
Acq On : 05 Oct 2021 11:25
Operator : SY/MD
Sample : M3967-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0S8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022563.D
Acq On : 05 Oct 2021 11:25
Operator : SY/MD
Sample : M3967-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0S8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
