

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022568.D
 Acq On : 05 Oct 2021 13:25
 Operator : SY/MD
 Sample : M3967-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0T3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	71	rVB3	6588	9132	2.41%	0.304%
2	1.304	76	82	91	rVB	27302	26701	7.04%	0.889%
3	1.564	156	163	174	rBV	41220	44015	11.61%	1.466%
4	1.748	211	220	231	rBV	39827	52123	13.75%	1.736%
5	2.114	319	334	354	rBV3	216272	347485	91.66%	11.572%
6	2.773	530	539	554	rVB3	3203	6700	1.77%	0.223%
7	3.896	876	888	923	rBV	44605	161170	42.51%	5.367%
8	4.349	1012	1029	1057	rBV2	54032	146786	38.72%	4.888%
9	5.047	1231	1246	1271	rBV2	119885	299046	78.88%	9.959%
10	5.619	1412	1424	1448	rBV	109814	225200	59.40%	7.500%
11	5.915	1503	1516	1532	rVB7	5293	12528	3.30%	0.417%
12	6.072	1552	1565	1590	rBV	73996	152686	40.28%	5.085%
13	6.992	1840	1851	1872	rBV2	23445	44740	11.80%	1.490%
14	7.317	1939	1952	1972	rBV	122927	214965	56.70%	7.159%
15	7.625	2040	2048	2063	rBV3	14344	24590	6.49%	0.819%
16	8.092	2183	2193	2228	rBV3	188733	379108	100.00%	12.625%
17	8.854	2419	2430	2455	rBV	173350	285658	75.35%	9.513%
18	10.217	2843	2854	2868	rBV	57822	92687	24.45%	3.087%
19	11.249	3165	3175	3195	rBV	166497	261156	68.89%	8.697%
20	11.625	3281	3292	3310	rBV	137121	216279	57.05%	7.203%




Sum of corrected areas: 3002755

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022568.D
Acq On : 05 Oct 2021 13:25
Operator : SY/MD
Sample : M3967-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

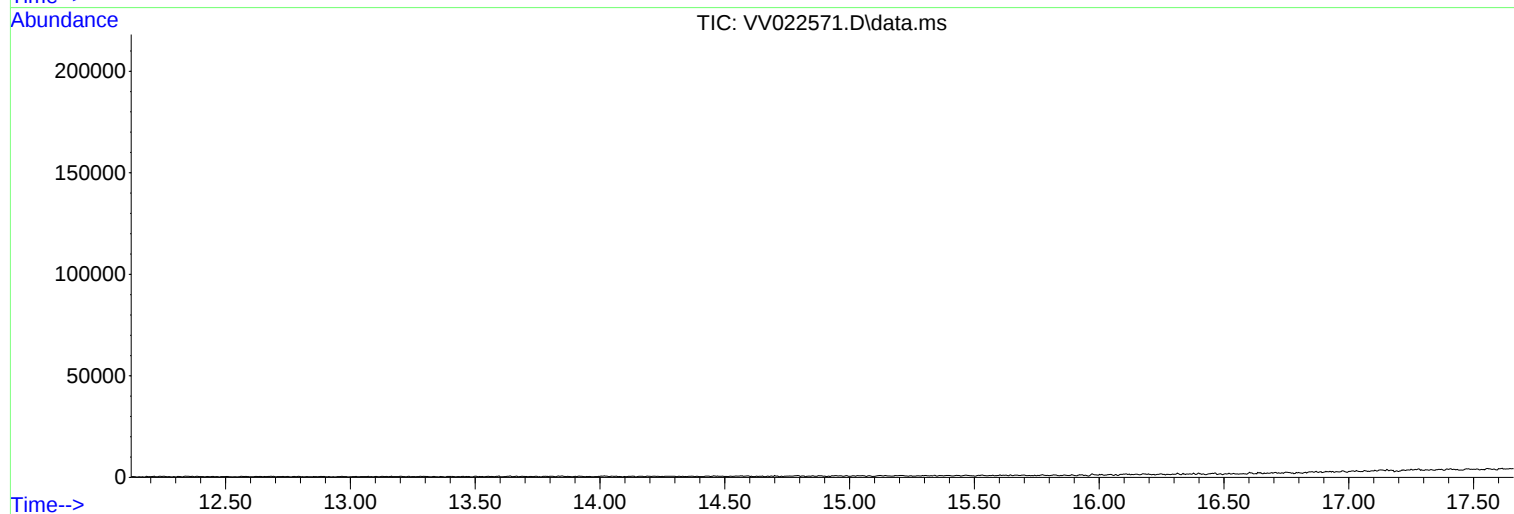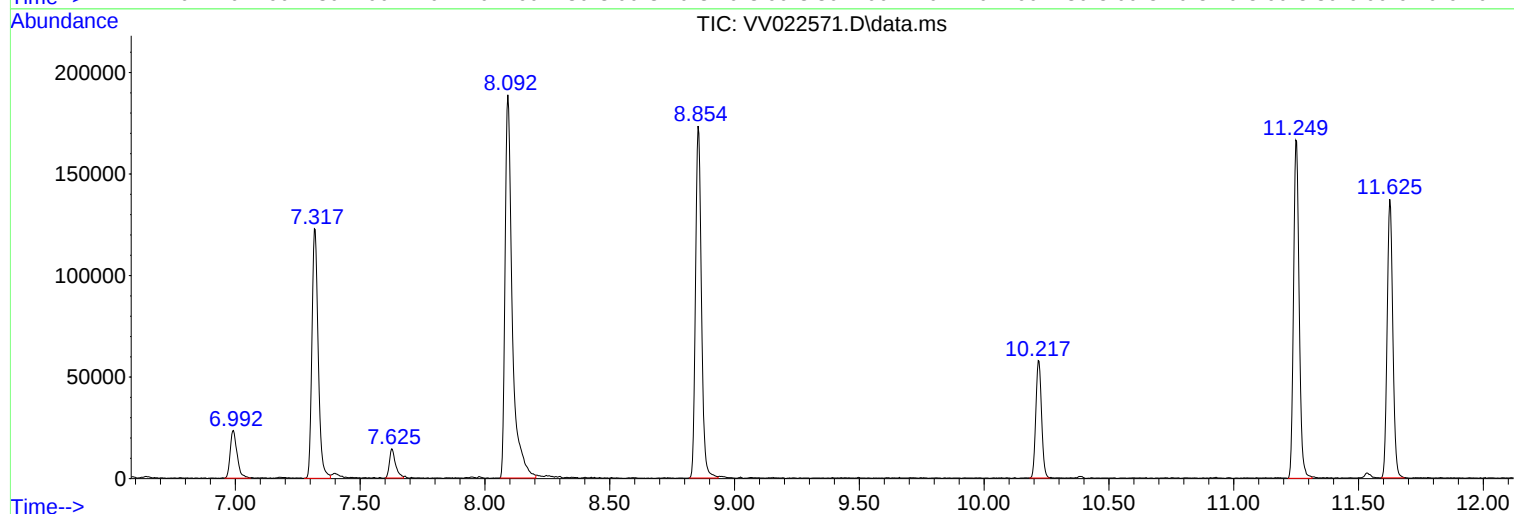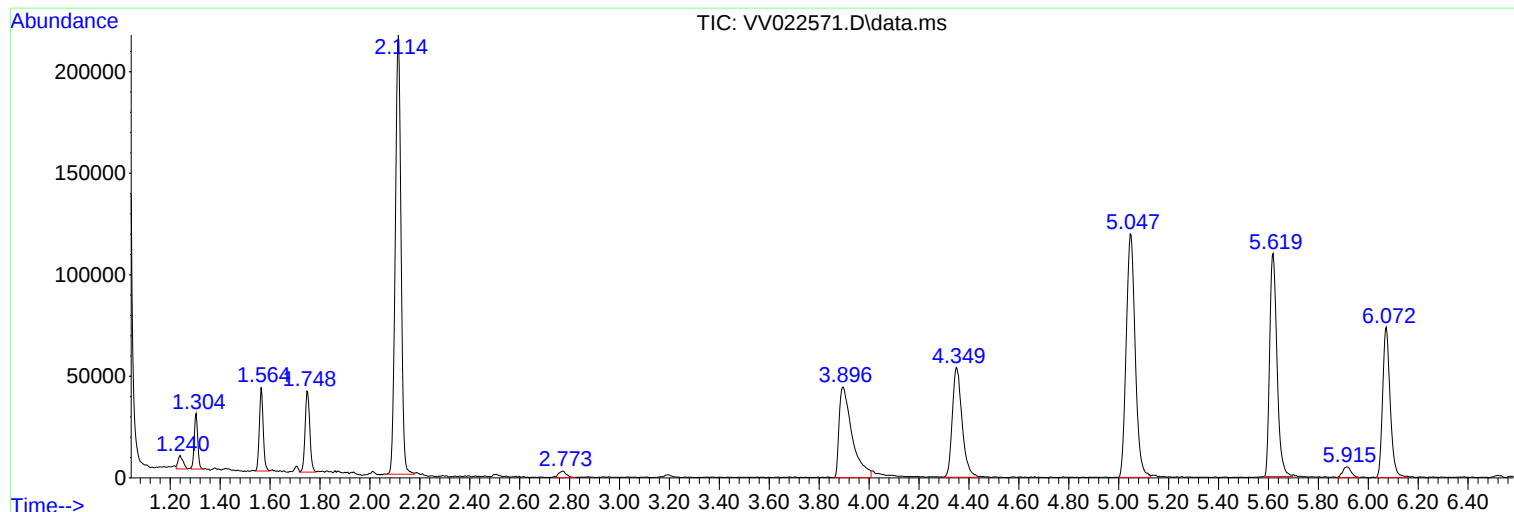

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022568.D
Acq On : 05 Oct 2021 13:25
Operator : SY/MD
Sample : M3967-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022568.D
Acq On : 05 Oct 2021 13:25
Operator : SY/MD
Sample : M3967-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
