

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022569.D
 Acq On : 05 Oct 2021 13:49
 Operator : SY/MD
 Sample : M3967-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0T4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB	27984	29471	8.09%	1.114%
2	1.564	155	163	173	rBV	39249	43850	12.04%	1.658%
3	2.105	319	331	343	rBV	62344	91038	24.99%	3.442%
4	2.166	345	350	364	rVB2	2995	4896	1.34%	0.185%
5	3.879	873	883	918	rBV2	55934	158055	43.38%	5.977%
6	4.352	1014	1030	1053	rBV	53156	137105	37.63%	5.184%
7	5.047	1231	1246	1275	rBV2	116425	296788	81.46%	11.223%
8	5.619	1411	1424	1446	rBV	113156	228330	62.67%	8.634%
9	5.915	1501	1516	1528	rBV9	5478	11993	3.29%	0.454%
10	6.069	1552	1564	1585	rBV	70722	148633	40.80%	5.620%
11	6.989	1838	1850	1865	rBV2	22743	42493	11.66%	1.607%
12	7.317	1941	1952	1973	rBV	120186	211977	58.18%	8.016%
13	7.628	2038	2049	2062	rBV2	13704	24734	6.79%	0.935%
14	8.088	2181	2192	2225	rBV2	183636	364323	100.00%	13.776%
15	8.853	2419	2430	2451	rBV	173015	284007	77.95%	10.739%
16	10.217	2844	2854	2865	rBV	57881	89970	24.70%	3.402%
17	11.249	3164	3175	3195	rBV	165134	258130	70.85%	9.761%
18	11.532	3254	3263	3271	rBV6	2786	4426	1.21%	0.167%
19	11.625	3281	3292	3309	rBV	138444	214321	58.83%	8.104%




Sum of corrected areas: 2644540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022569.D
Acq On : 05 Oct 2021 13:49
Operator : SY/MD
Sample : M3967-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG0T4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

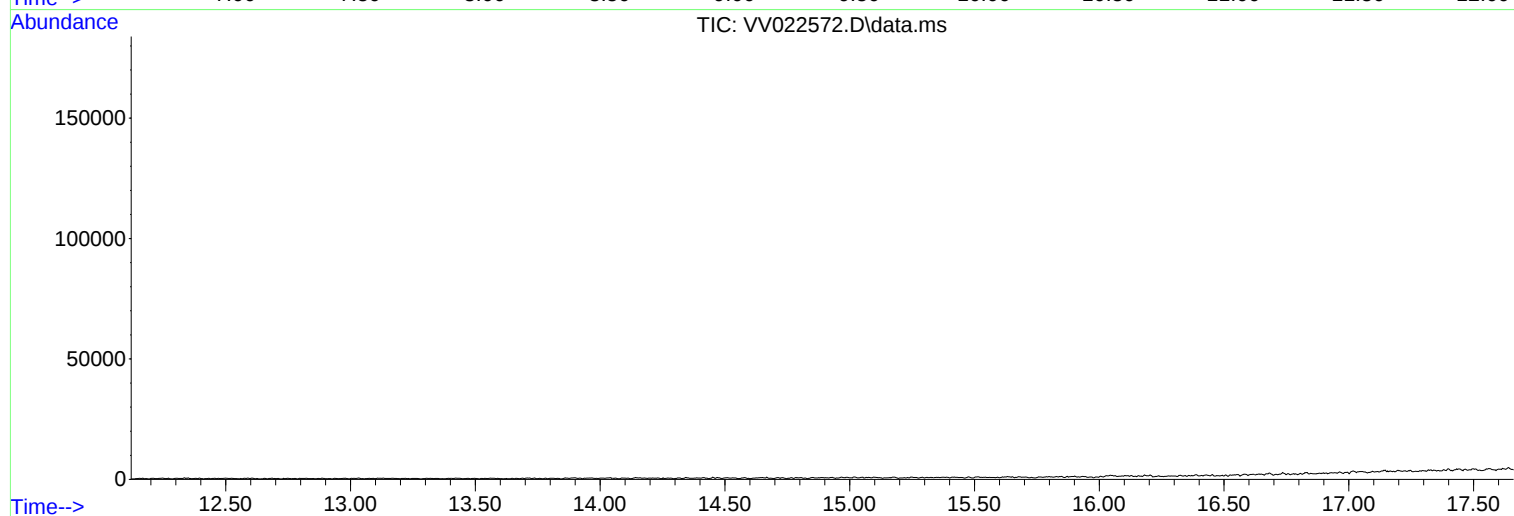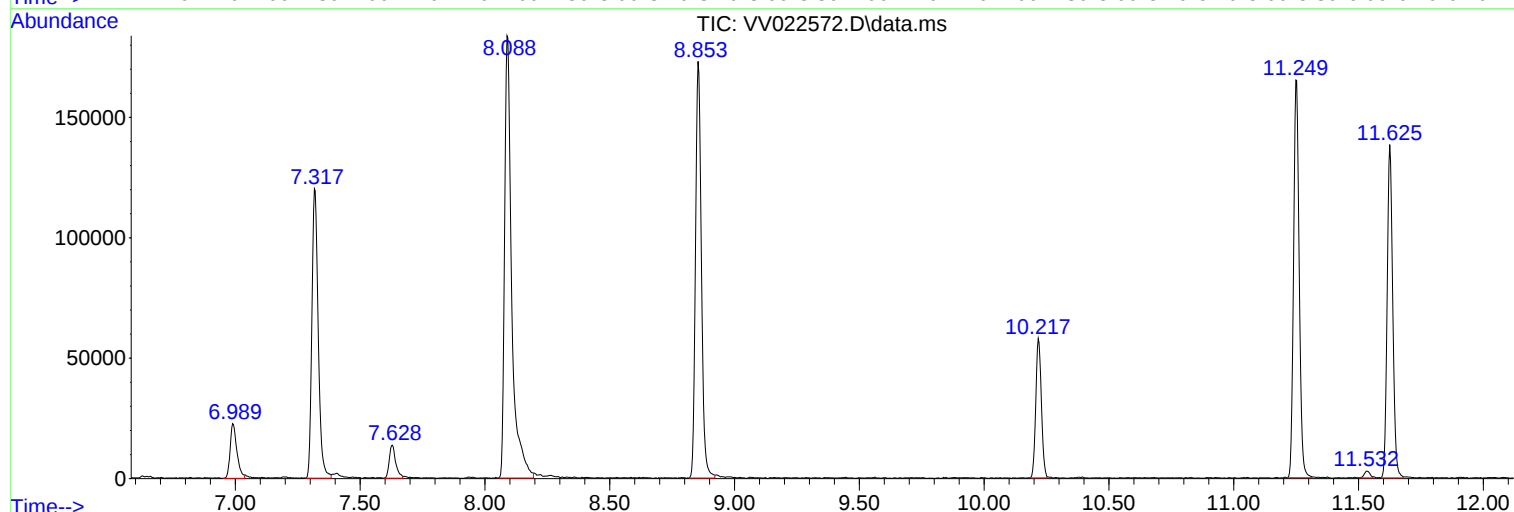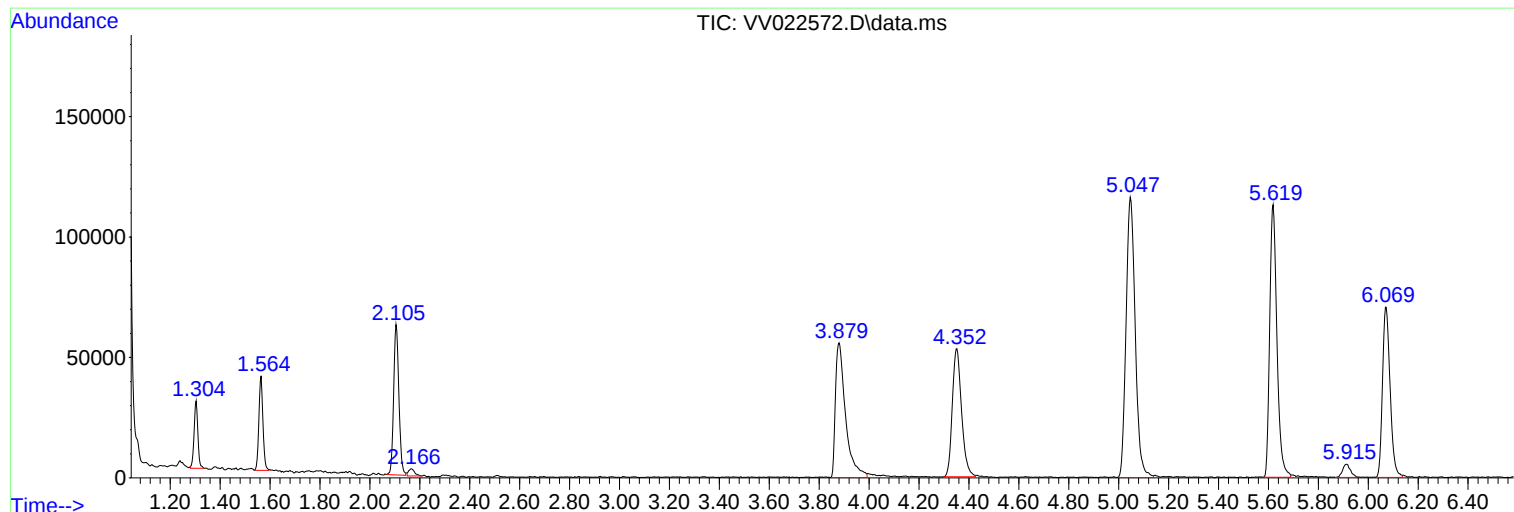

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022569.D
Acq On : 05 Oct 2021 13:49
Operator : SY/MD
Sample : M3967-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022569.D
Acq On : 05 Oct 2021 13:49
Operator : SY/MD
Sample : M3967-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
