

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022571.D
 Acq On : 05 Oct 2021 14:38
 Operator : SY/MD
 Sample : M3967-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG0T7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.236	57	61	74	rVB2	3939	5996	1.52%	0.214%
2	1.304	76	82	90	rVV	29397	27961	7.09%	0.996%
3	1.564	156	163	172	rBV	40899	45283	11.49%	1.613%
4	1.941	274	280	290	rVB6	3867	5761	1.46%	0.205%
5	2.104	320	331	347	rBV3	77397	127196	32.26%	4.531%
6	2.770	525	538	553	rBV3	10581	23089	5.86%	0.823%
7	3.902	878	890	924	rBV2	45795	174759	44.33%	6.226%
8	4.352	1014	1030	1051	rBV2	52273	138666	35.17%	4.940%
9	5.046	1230	1246	1273	rBV3	121715	304455	77.22%	10.846%
10	5.619	1412	1424	1446	rBV	109507	224773	57.01%	8.008%
11	5.918	1506	1517	1527	rBV10	8140	19028	4.83%	0.678%
12	6.072	1548	1565	1581	rBV2	75390	153153	38.85%	5.456%
13	6.992	1841	1851	1867	rBV	23524	43735	11.09%	1.558%
14	7.320	1941	1953	1972	rBV	122651	217025	55.05%	7.732%
15	7.628	2037	2049	2065	rBV	13831	26656	6.76%	0.950%
16	7.979	2147	2158	2168	rVB3	13664	22927	5.82%	0.817%
17	8.091	2183	2193	2226	rBV2	193079	394255	100.00%	14.046%
18	8.853	2419	2430	2451	rBV	171474	279980	71.01%	9.974%
19	10.220	2844	2855	2869	rBV	61933	96466	24.47%	3.437%
20	11.252	3165	3176	3195	rBV	160098	251944	63.90%	8.976%
21	11.625	3279	3292	3311	rBV	140960	223857	56.78%	7.975%




Sum of corrected areas: 2806965

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022571.D
Acq On : 05 Oct 2021 14:38
Operator : SY/MD
Sample : M3967-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

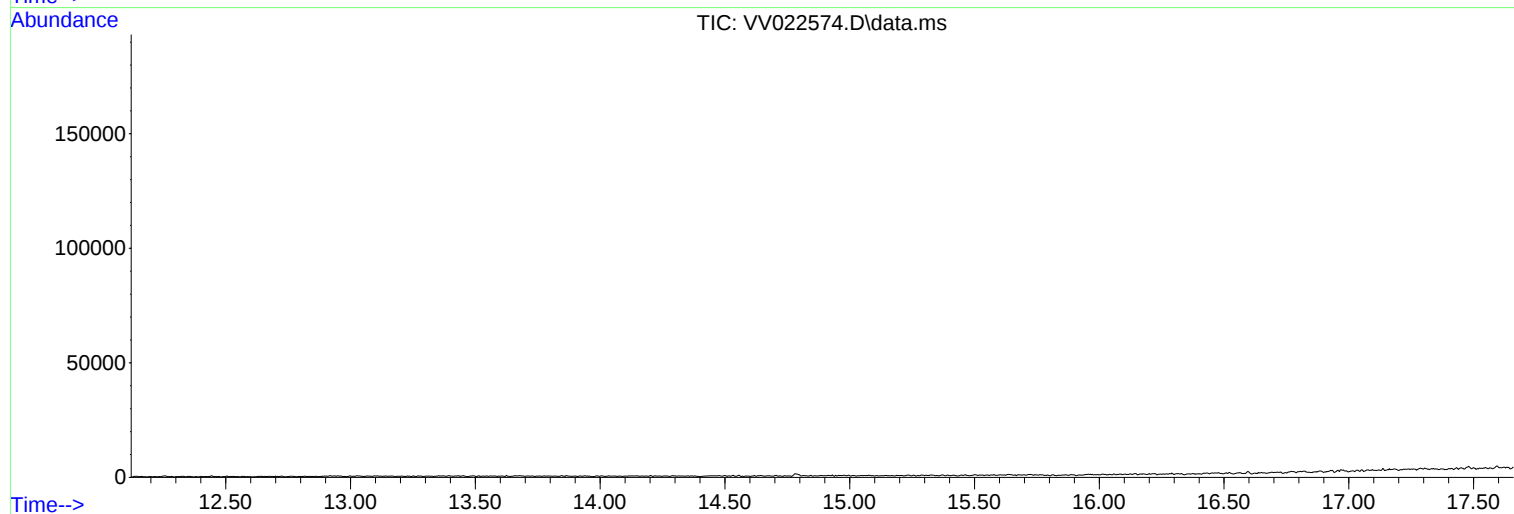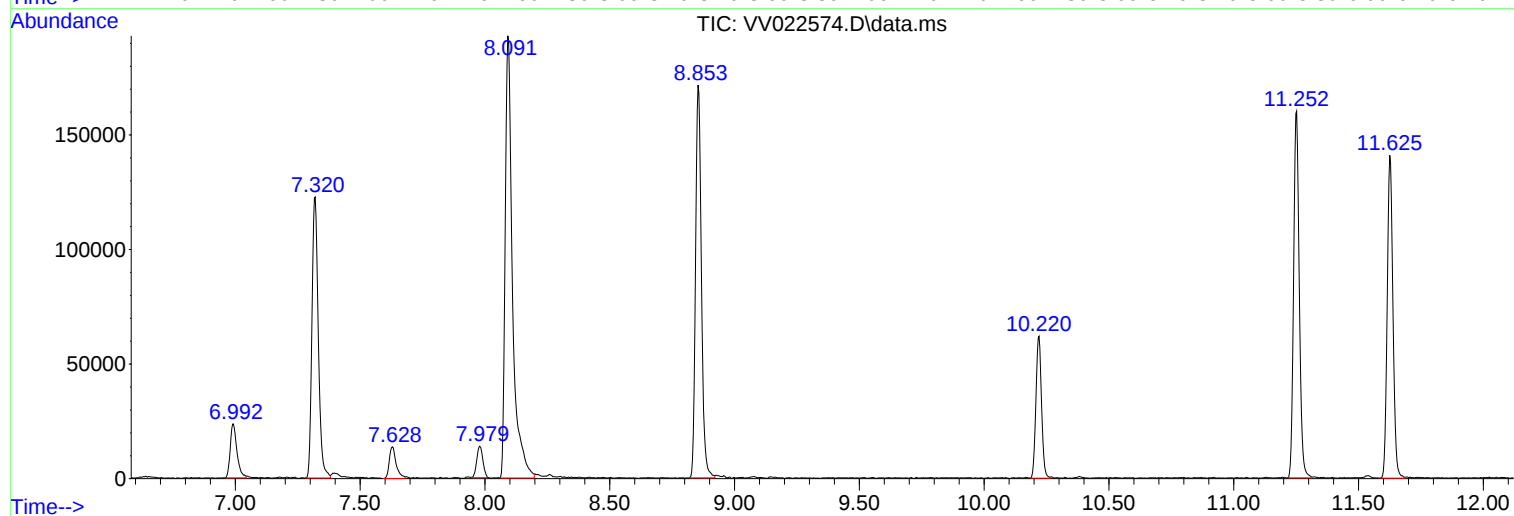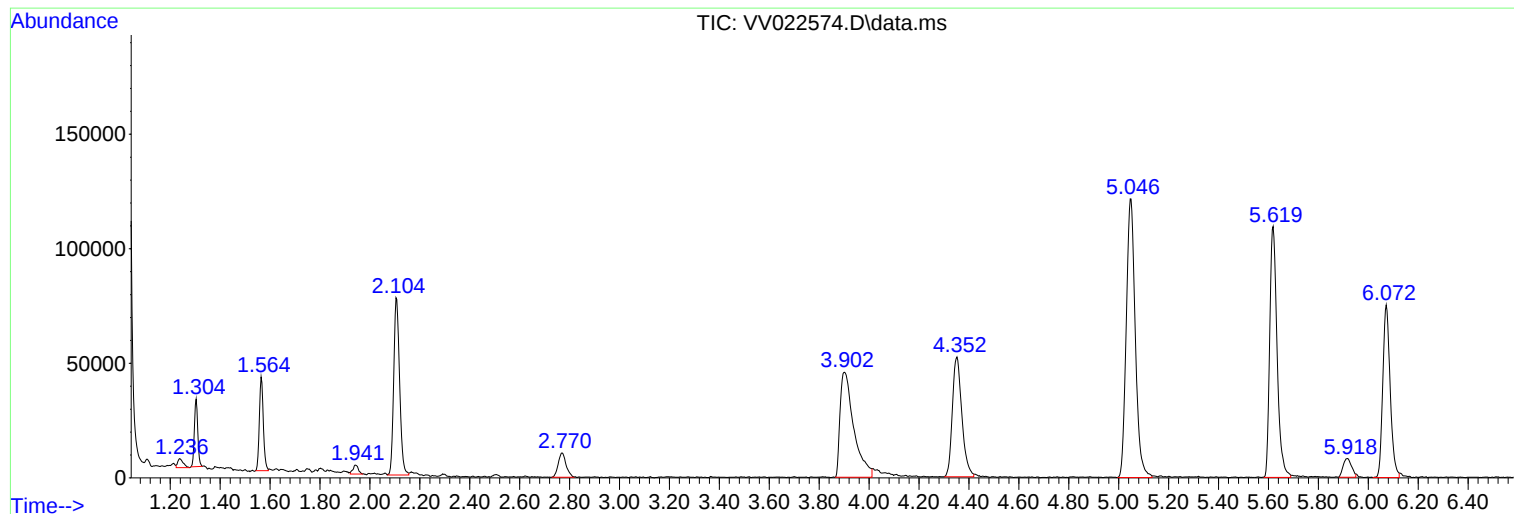

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022571.D
Acq On : 05 Oct 2021 14:38
Operator : SY/MD
Sample : M3967-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022571.D
Acq On : 05 Oct 2021 14:38
Operator : SY/MD
Sample : M3967-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG0T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
