

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022573.D
 Acq On : 05 Oct 2021 15:26
 Operator : SY/MD
 Sample : M4052-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB2	31059	32347	4.08%	0.801%
2	1.565	156	163	174	rVB	38228	43504	5.49%	1.077%
3	1.947	273	282	292	rVB2	16733	25178	3.18%	0.623%
4	2.108	321	332	347	rBV3	76769	129571	16.35%	3.208%
5	2.770	522	538	553	rBV2	25761	55905	7.05%	1.384%
6	3.912	875	893	931	rBV2	293649	792617	100.00%	19.627%
7	4.352	1014	1030	1055	rBV2	51818	134455	16.96%	3.329%
8	5.050	1231	1247	1268	rBV2	113291	283000	35.70%	7.008%
9	5.619	1412	1424	1444	rBV	105396	211288	26.66%	5.232%
10	5.915	1501	1516	1545	rBV	303818	597928	75.44%	14.806%
11	6.072	1553	1565	1584	rBV2	70186	143927	18.16%	3.564%
12	6.992	1841	1851	1871	rBV	23243	43618	5.50%	1.080%
13	7.320	1941	1953	1972	rBV	110404	196118	24.74%	4.856%
14	7.629	2039	2049	2063	rBV3	13616	23816	3.00%	0.590%
15	7.979	2145	2158	2178	rVB	79516	135511	17.10%	3.356%
16	8.092	2182	2193	2233	rBV2	183809	381750	48.16%	9.453%
17	8.854	2418	2430	2455	rBV	159672	262688	33.14%	6.505%
18	10.217	2844	2854	2871	rBV	58268	91093	11.49%	2.256%
19	11.252	3165	3176	3194	rBV	151733	238411	30.08%	5.903%
20	11.625	3277	3292	3313	rBV	131193	215747	27.22%	5.342%




Sum of corrected areas: 4038472

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022573.D
Acq On : 05 Oct 2021 15:26
Operator : SY/MD
Sample : M4052-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

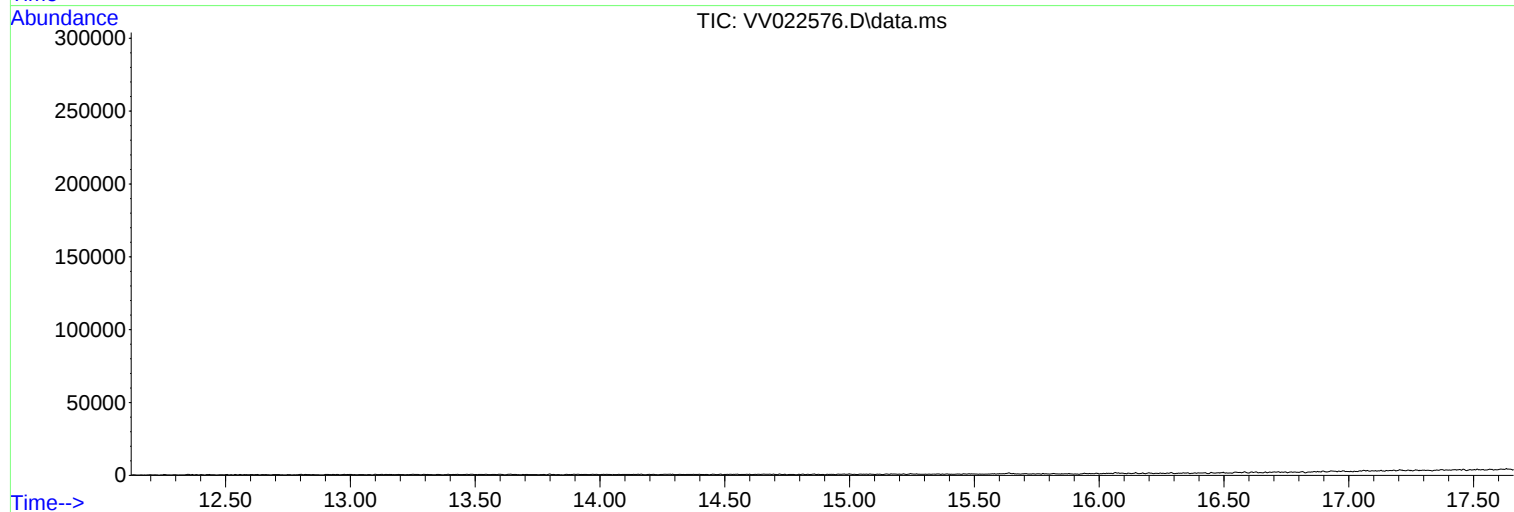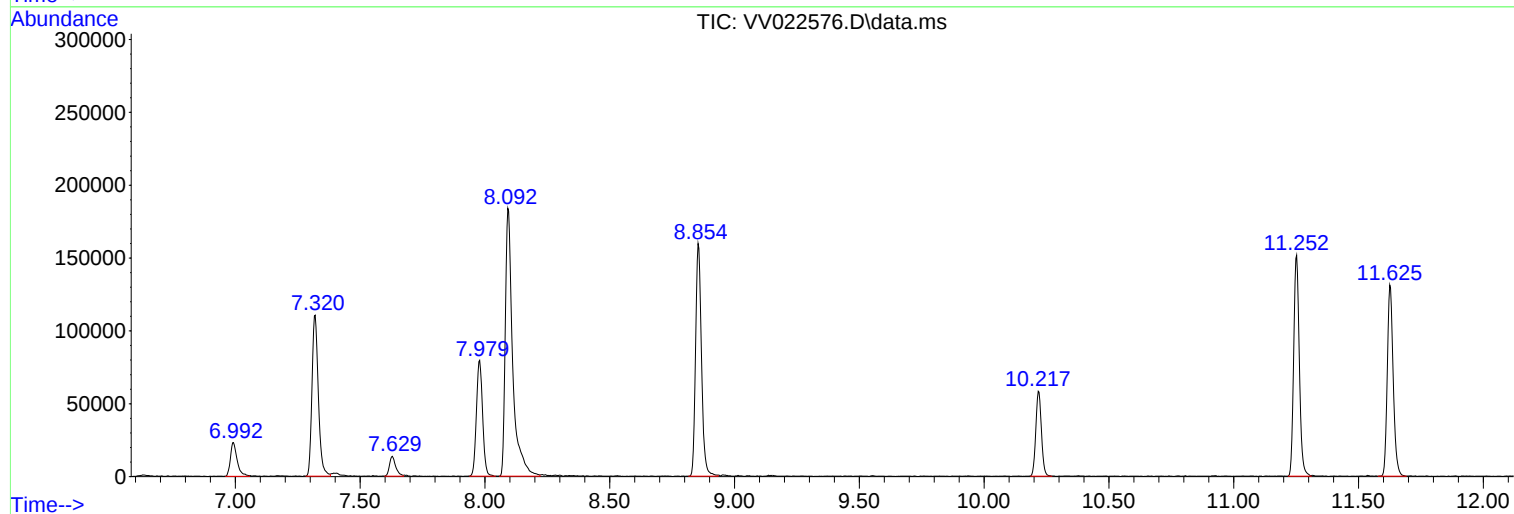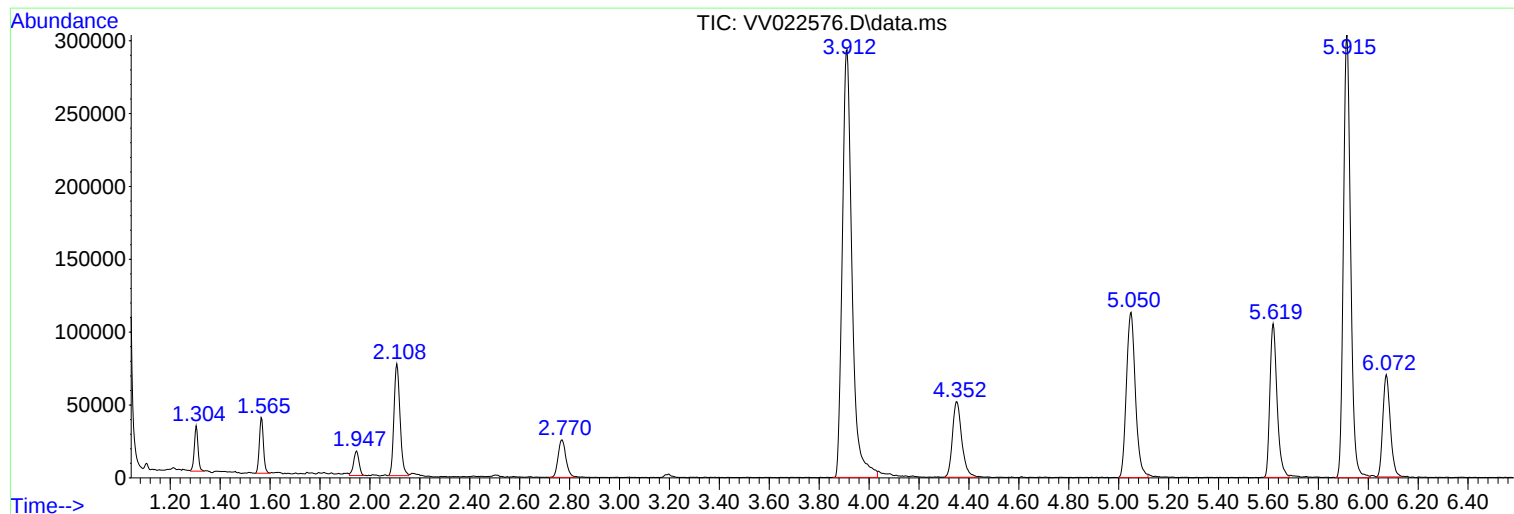

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022573.D
Acq On : 05 Oct 2021 15:26
Operator : SY/MD
Sample : M4052-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX1









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.947	0.60 ug/L	25178	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	49
2			2-Pentyn-4-one	82	C5H6O	007299-55-0	9
3			1,3-Isobenzofurandione, hexahydr...	154	C8H10O3	014166-21-3	9
4			Cyclopropane, 1,2-dimethyl-3-met...	82	C6H10	004866-55-1	9
5			1,3-Butadiene, 2-(bromomethyl)-	146	C5H7Br	023691-13-6	9

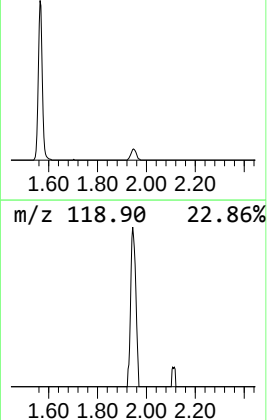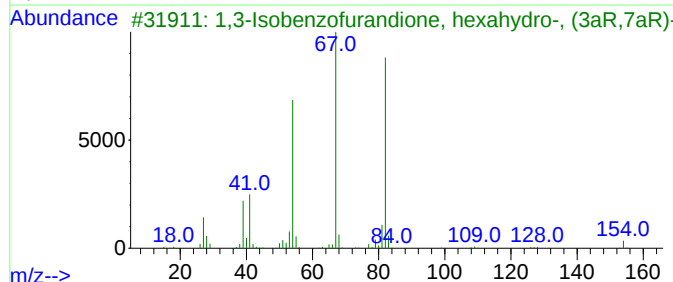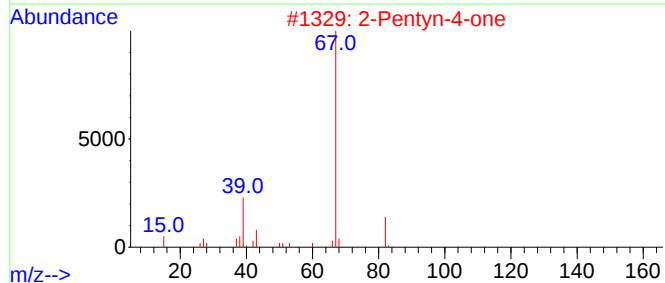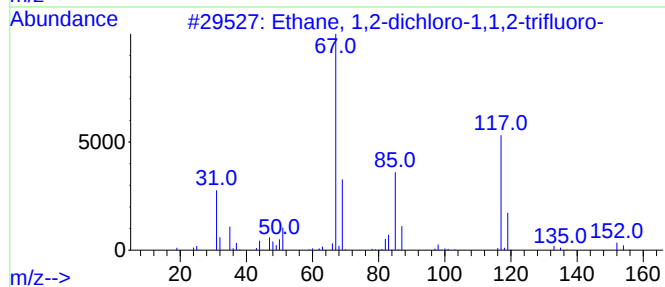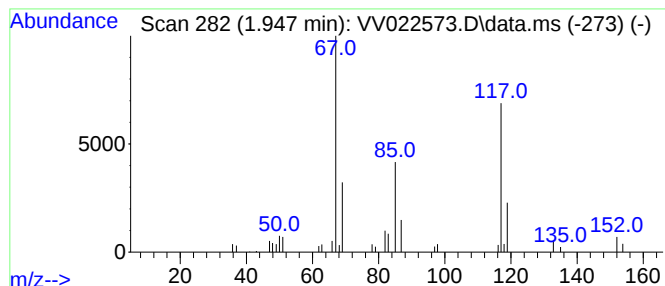

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022573.D
Acq On : 05 Oct 2021 15:26
Operator : SY/MD
Sample : M4052-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.947	0.6	ug/L	25178	1	5.619	211288	5.0