

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022578.D
 Acq On : 05 Oct 2021 17:26
 Operator : SY/MD
 Sample : M4052-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	27	rVB	7828	6786	1.80%	0.218%
2	1.304	74	82	95	rBV	62628	67033	17.80%	2.149%
3	1.561	153	162	177	rBV	57283	66536	17.67%	2.133%
4	2.105	318	331	344	rBV	111219	163589	43.44%	5.244%
5	2.156	344	347	359	rVB2	4038	5437	1.44%	0.174%
6	2.291	377	389	400	rBV4	2573	4717	1.25%	0.151%
7	2.767	525	537	548	rBV10	2989	5931	1.57%	0.190%
8	3.876	872	882	917	rBV	49888	142601	37.87%	4.571%
9	4.349	1013	1029	1054	rBV2	65349	164662	43.73%	5.278%
10	5.047	1230	1246	1268	rBV2	150734	376578	100.00%	12.071%
11	5.619	1409	1424	1445	rBV	114526	232111	61.64%	7.440%
12	5.918	1505	1517	1532	rBV7	14461	32026	8.50%	1.027%
13	6.072	1551	1565	1585	rBV2	86824	176694	46.92%	5.664%
14	6.989	1840	1850	1866	rBV2	33016	60199	15.99%	1.930%
15	7.317	1941	1952	1969	rBV	178009	312767	83.06%	10.026%
16	7.397	1969	1977	1991	rVB	8712	16559	4.40%	0.531%
17	7.625	2036	2048	2067	rBV2	19487	34886	9.26%	1.118%
18	8.088	2183	2192	2226	rBV3	156158	324553	86.18%	10.403%
19	8.854	2419	2430	2449	rBV	178428	287605	76.37%	9.219%
20	9.146	2512	2521	2533	rBV3	3469	5710	1.52%	0.183%
21	10.217	2843	2854	2871	rBV	59437	92822	24.65%	2.975%
22	11.249	3164	3175	3193	rBV	169629	266660	70.81%	8.548%
23	11.625	3280	3292	3307	rBV	174055	273244	72.56%	8.759%




Sum of corrected areas: 3119706

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022578.D
Acq On : 05 Oct 2021 17:26
Operator : SY/MD
Sample : M4052-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

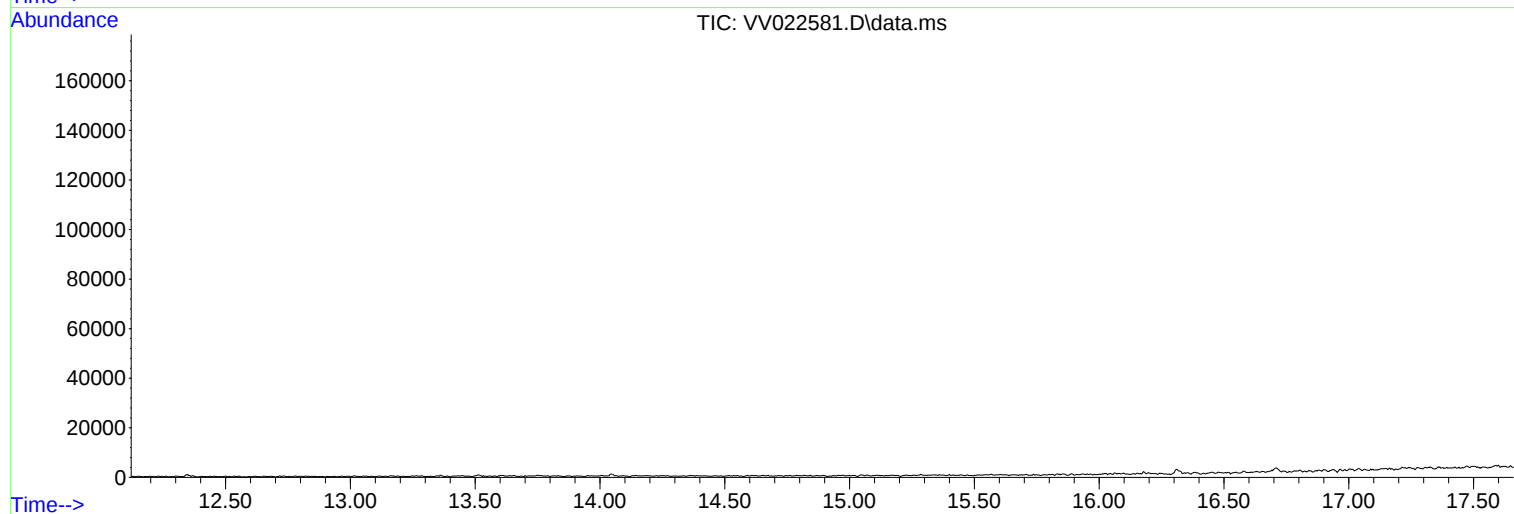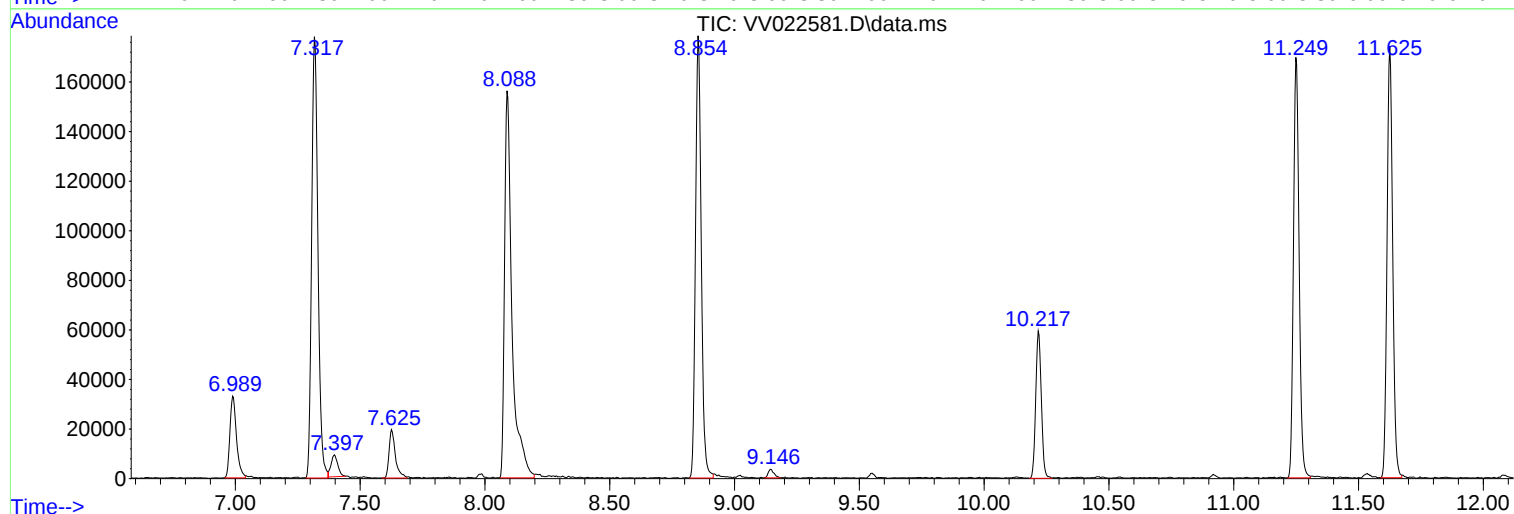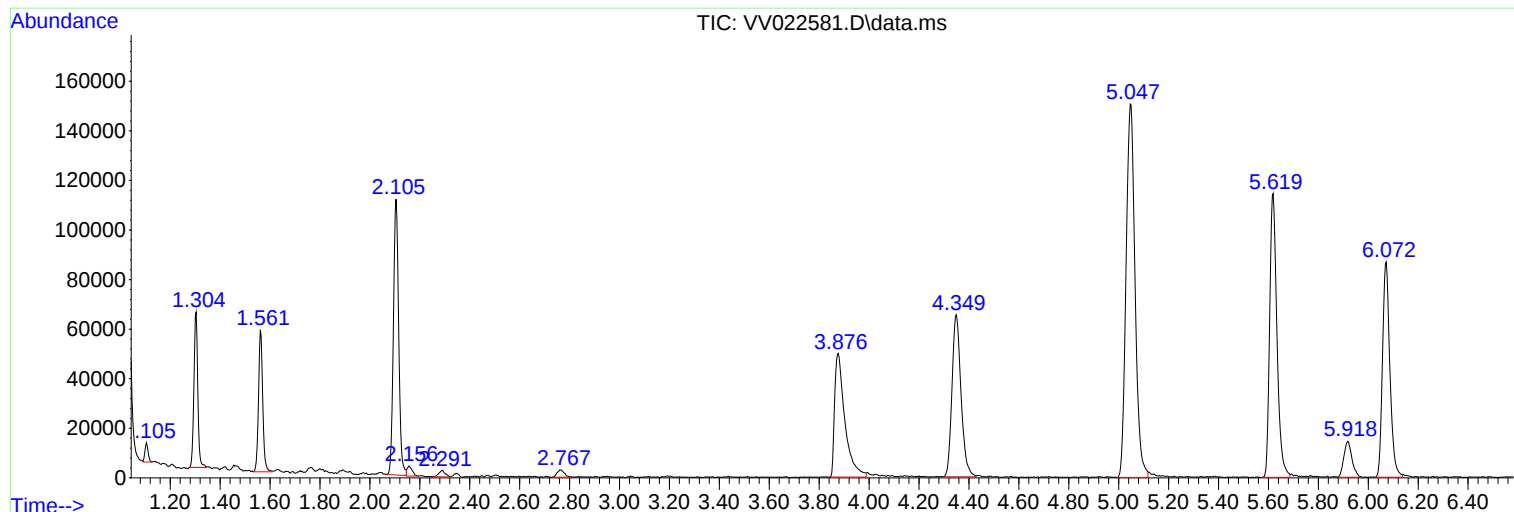

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022578.D
Acq On : 05 Oct 2021 17:26
Operator : SY/MD
Sample : M4052-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022578.D
Acq On : 05 Oct 2021 17:26
Operator : SY/MD
Sample : M4052-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
