

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022579.D
 Acq On : 05 Oct 2021 17:51
 Operator : SY/MD
 Sample : M4052-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	94	rBV	61787	62919	16.49%	1.861%
2	1.565	155	163	173	rBV	54777	61805	16.20%	1.828%
3	2.105	321	331	345	rBV2	113024	169444	44.41%	5.011%
4	2.291	378	389	405	rBV	118289	176008	46.13%	5.205%
5	3.908	875	892	930	rBV4	76840	270361	70.86%	7.995%
6	4.349	1013	1029	1062	rBV	67366	170033	44.57%	5.028%
7	5.047	1230	1246	1280	rBV2	153757	381524	100.00%	11.282%
8	5.619	1407	1424	1443	rBV	106034	219024	57.41%	6.477%
9	5.918	1505	1517	1541	rVB5	29550	64018	16.78%	1.893%
10	6.069	1551	1564	1586	rBV2	86183	177610	46.55%	5.252%
11	6.989	1839	1850	1869	rBV	33715	62402	16.36%	1.845%
12	7.240	1919	1928	1941	rBV4	6076	11698	3.07%	0.346%
13	7.317	1941	1952	1970	rBV	176611	308930	80.97%	9.135%
14	7.625	2038	2048	2068	rBV2	20137	36748	9.63%	1.087%
15	7.982	2150	2159	2169	rVB5	5317	8586	2.25%	0.254%
16	8.092	2182	2193	2230	rBV2	174182	344724	90.35%	10.194%
17	8.854	2418	2430	2448	rBV	161061	265705	69.64%	7.857%
18	10.217	2843	2854	2872	rVB	61008	94243	24.70%	2.787%
19	11.249	3165	3175	3194	rBV	151009	235942	61.84%	6.977%
20	11.625	3281	3292	3310	rBV	166680	259923	68.13%	7.686%




Sum of corrected areas: 3381647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022579.D
Acq On : 05 Oct 2021 17:51
Operator : SY/MD
Sample : M4052-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

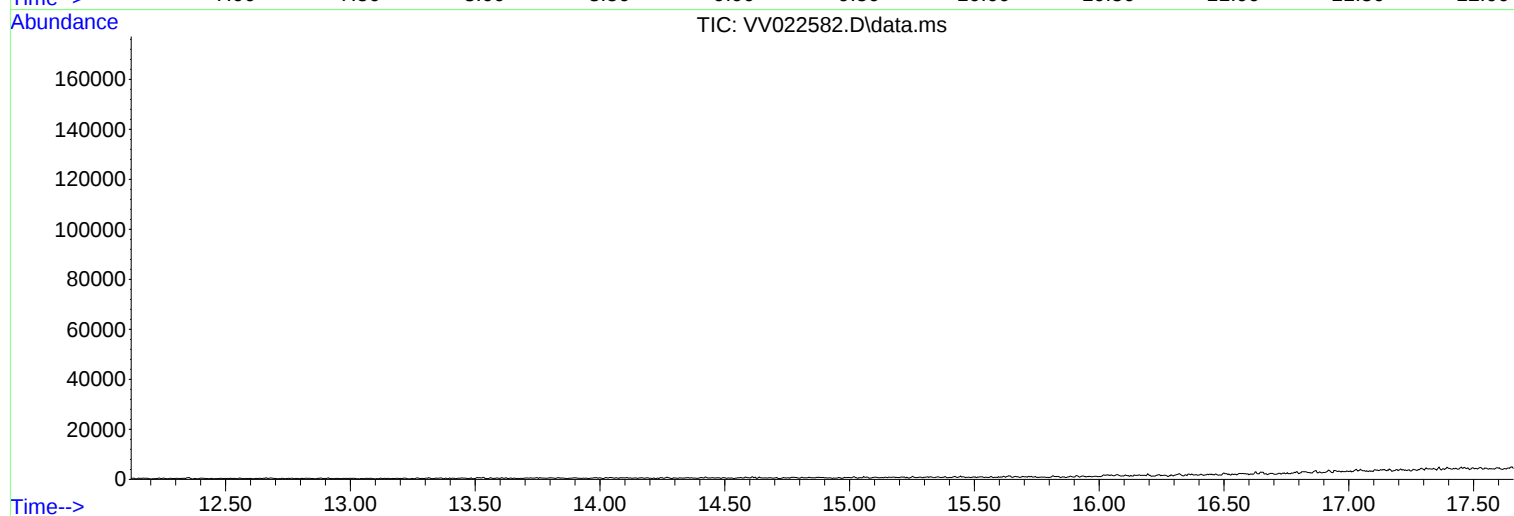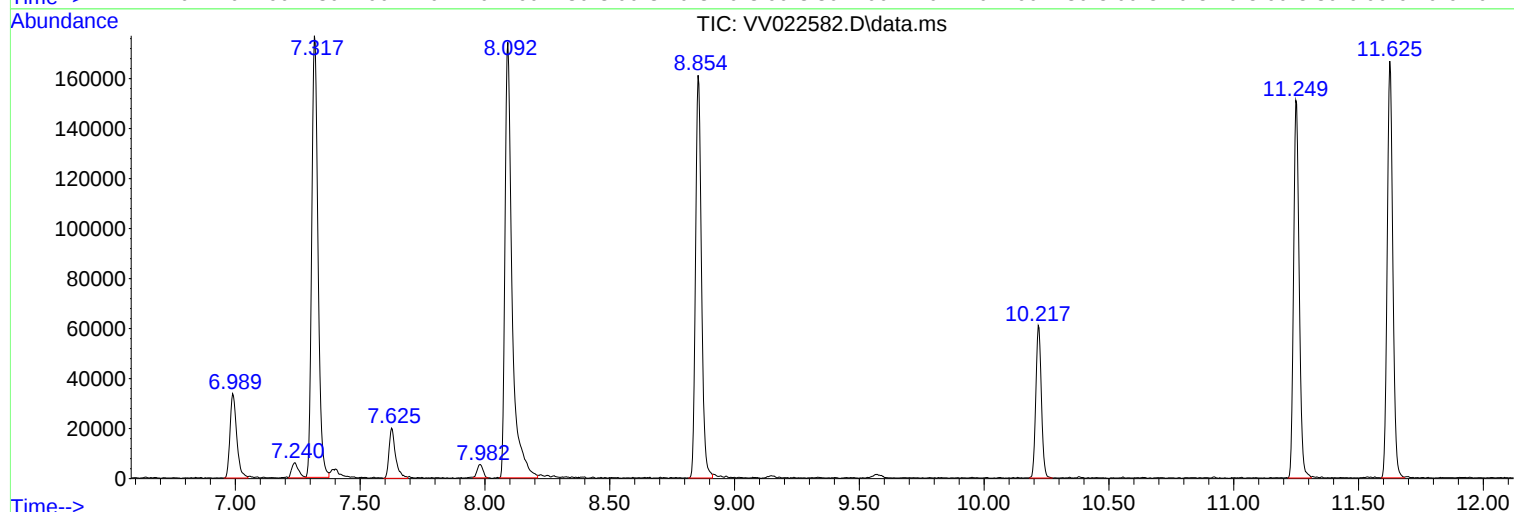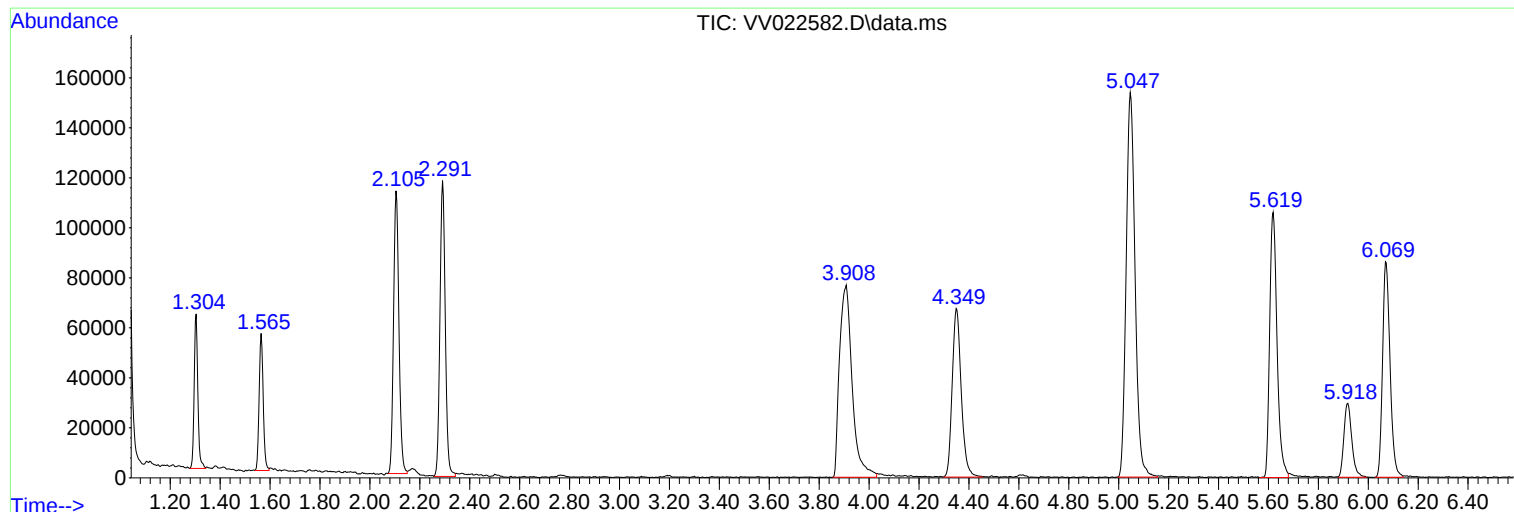

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022579.D
Acq On : 05 Oct 2021 17:51
Operator : SY/MD
Sample : M4052-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022579.D
Acq On : 05 Oct 2021 17:51
Operator : SY/MD
Sample : M4052-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
