

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022580.D
 Acq On : 05 Oct 2021 18:15
 Operator : SY/MD
 Sample : M4052-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	98	rVB	65532	68975	3.74%	1.006%
2	1.561	155	162	176	rVB	59113	66641	3.61%	0.972%
3	2.114	320	334	348	rBV3	370644	603335	32.72%	8.801%
4	3.192	657	669	684	rBV	15526	33470	1.82%	0.488%
5	3.909	871	892	919	rBV3	212306	617514	33.49%	9.008%
6	4.352	1013	1030	1055	rBV	69067	176003	9.55%	2.567%
7	4.613	1095	1111	1126	rBV3	8385	21221	1.15%	0.310%
8	5.047	1226	1246	1270	rBV2	156125	390113	21.16%	5.691%
9	5.619	1412	1424	1451	rBV	116020	237176	12.86%	3.460%
10	5.915	1502	1516	1545	rBV	467959	920855	49.94%	13.432%
11	6.072	1551	1565	1584	rBV2	87512	179262	9.72%	2.615%
12	6.989	1840	1850	1867	rBV	35597	65971	3.58%	0.962%
13	7.317	1941	1952	1970	rBV	186171	324849	17.62%	4.739%
14	7.625	2039	2048	2069	rBV	21051	37227	2.02%	0.543%
15	7.976	2139	2157	2180	rBV	1110875	1843829	100.00%	26.896%
16	8.088	2183	2192	2224	rVB	177907	339843	18.43%	4.957%
17	8.854	2419	2430	2452	rBV	178363	292390	15.86%	4.265%
18	10.217	2843	2854	2869	rBV	60469	95135	5.16%	1.388%
19	11.252	3165	3176	3195	rBV	167196	265576	14.40%	3.874%
20	11.625	3280	3292	3312	rBV	170422	276066	14.97%	4.027%




Sum of corrected areas: 6855451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022580.D
Acq On : 05 Oct 2021 18:15
Operator : SY/MD
Sample : M4052-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

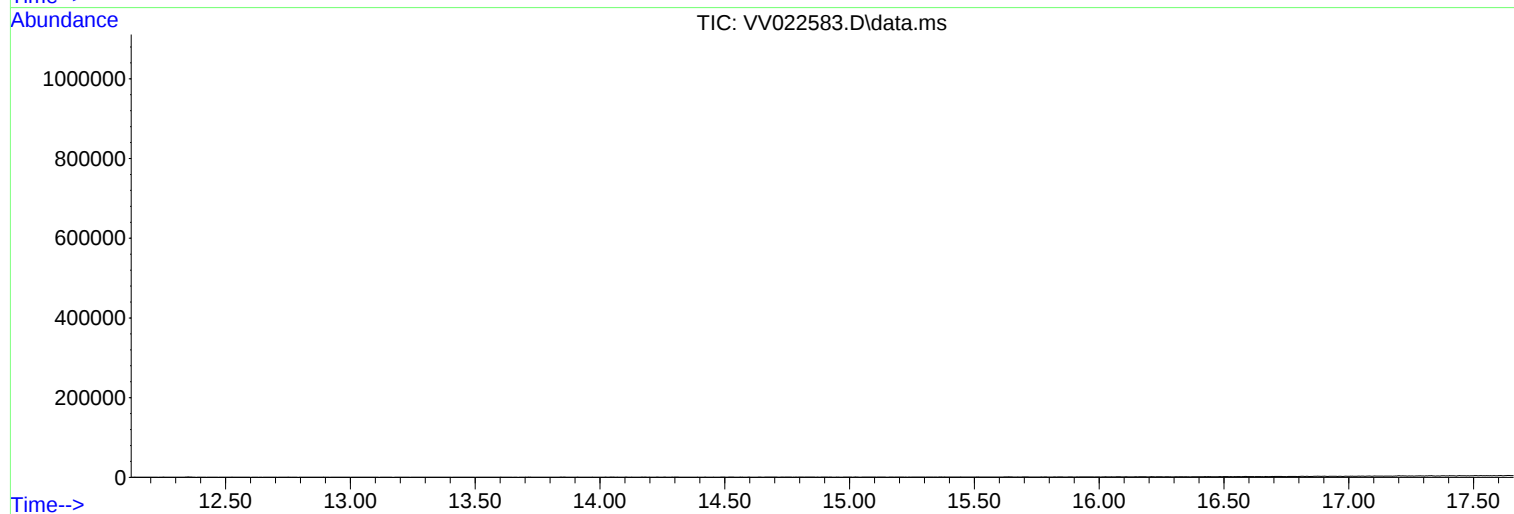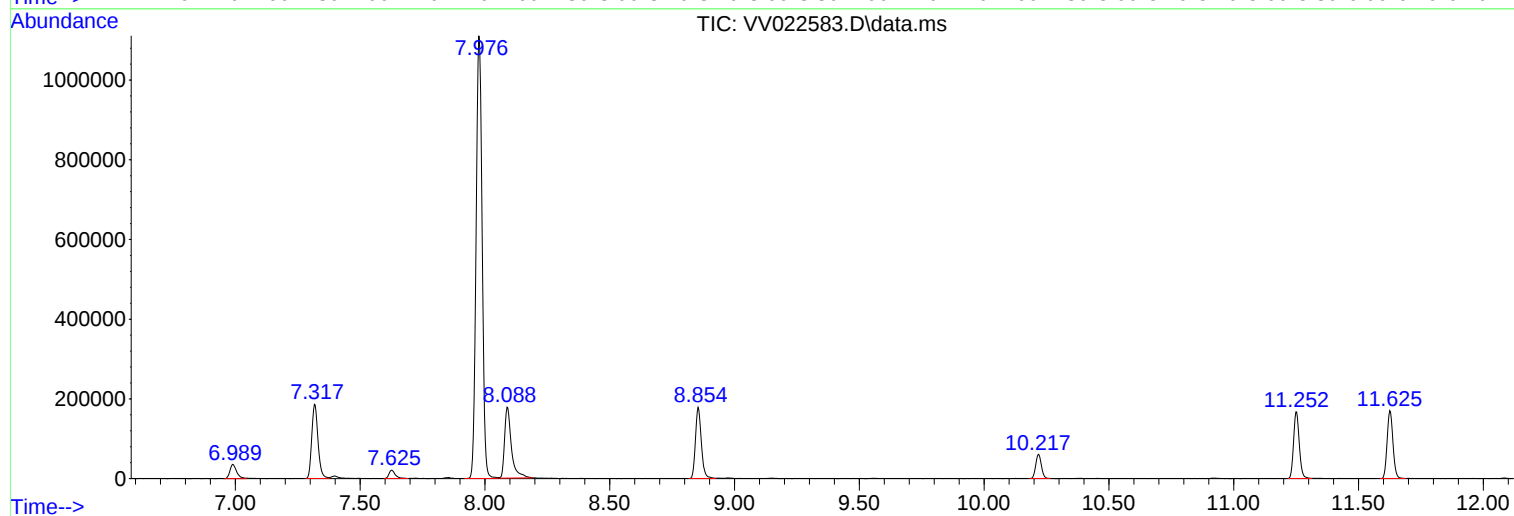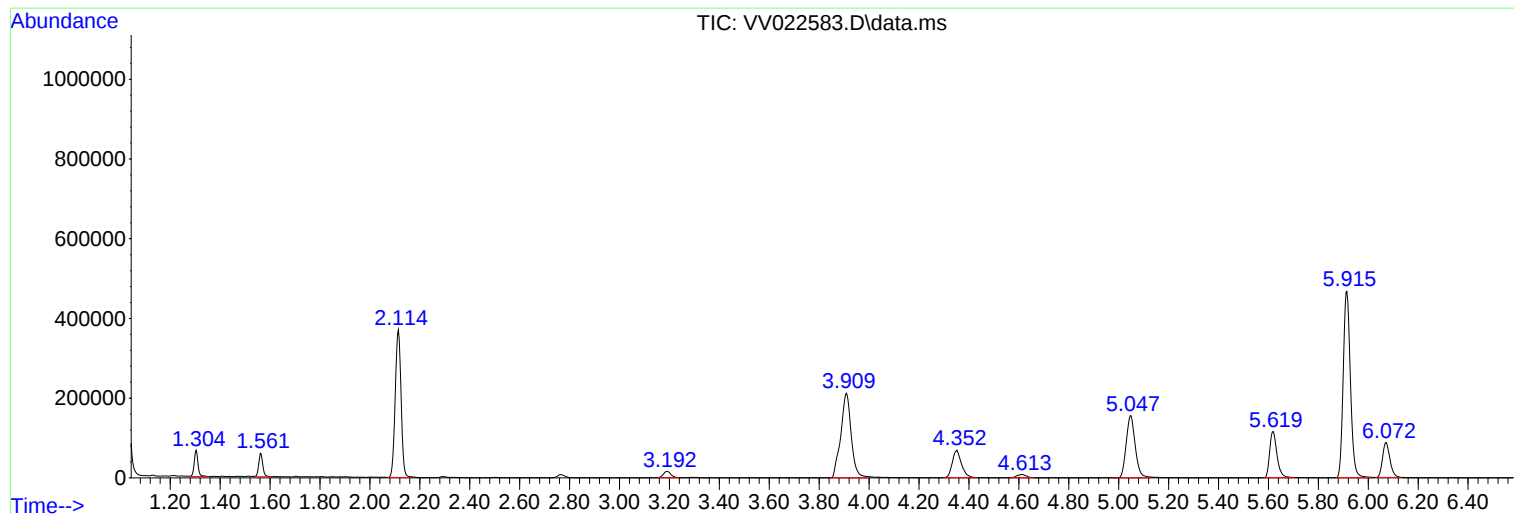

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022580.D
Acq On : 05 Oct 2021 18:15
Operator : SY/MD
Sample : M4052-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022580.D
Acq On : 05 Oct 2021 18:15
Operator : SY/MD
Sample : M4052-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
