

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022581.D
 Acq On : 05 Oct 2021 18:39
 Operator : SY/MD
 Sample : M4052-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rBV	60835	61073	15.86%	1.801%
2	1.564	155	163	174	rBV	58474	65528	17.02%	1.932%
3	1.751	214	221	228	rVB2	3993	4777	1.24%	0.141%
4	2.105	321	331	346	rBV2	117280	171829	44.63%	5.066%
5	3.902	876	890	920	rBV	37829	141786	36.82%	4.180%
6	4.352	1013	1030	1053	rBV2	62918	170357	44.25%	5.023%
7	4.825	1164	1177	1189	rBV6	3022	7138	1.85%	0.210%
8	5.047	1231	1246	1271	rBV2	156546	385029	100.00%	11.352%
9	5.619	1412	1424	1446	rBV	117514	237142	61.59%	6.992%
10	5.918	1503	1517	1534	rBV6	28614	61674	16.02%	1.818%
11	6.072	1551	1565	1586	rBV2	87662	181293	47.09%	5.345%
12	6.989	1840	1850	1871	rBV2	33680	62882	16.33%	1.854%
13	7.317	1940	1952	1968	rBV	183268	319551	82.99%	9.421%
14	7.394	1971	1976	1988	rVB	7048	11763	3.06%	0.347%
15	7.625	2038	2048	2065	rBV2	20099	36526	9.49%	1.077%
16	7.976	2145	2157	2180	rVB	119726	207148	53.80%	6.107%
17	8.091	2183	2193	2227	rBV2	168348	344409	89.45%	10.154%
18	8.854	2419	2430	2451	rBV	175183	288595	74.95%	8.509%
19	10.217	2842	2854	2869	rBV2	62663	97999	25.45%	2.889%
20	11.252	3164	3176	3197	rBV	168146	262223	68.10%	7.731%
21	11.625	3281	3292	3313	rBV	175669	273104	70.93%	8.052%




Sum of corrected areas: 3391826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022581.D
Acq On : 05 Oct 2021 18:39
Operator : SY/MD
Sample : M4052-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

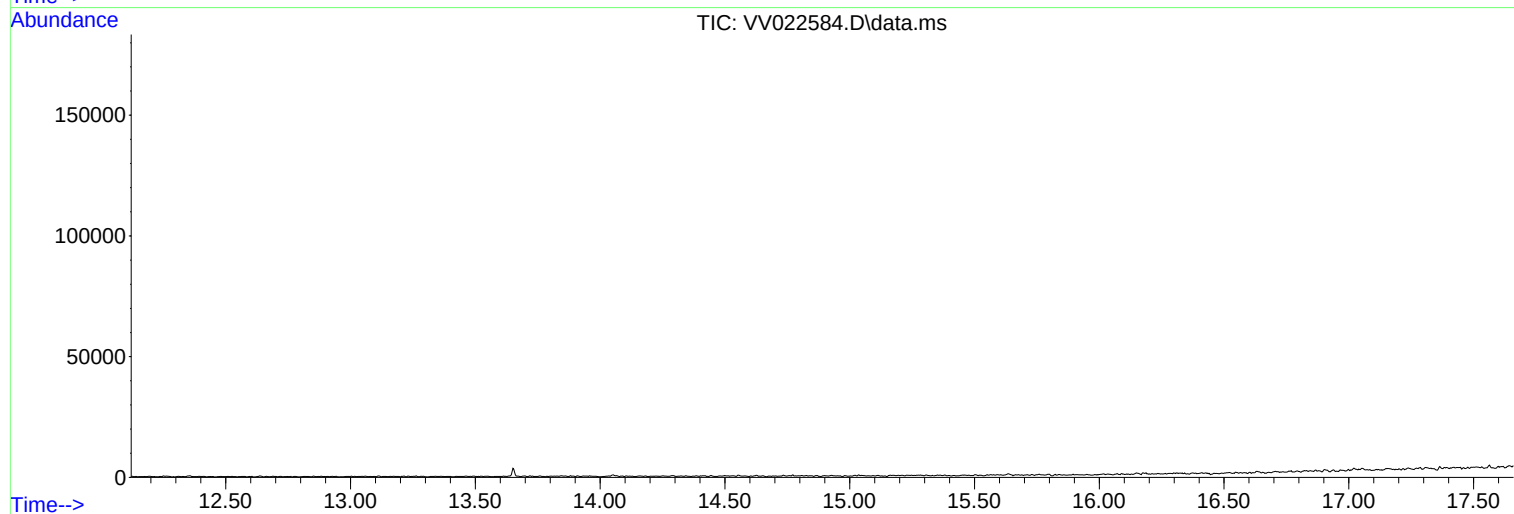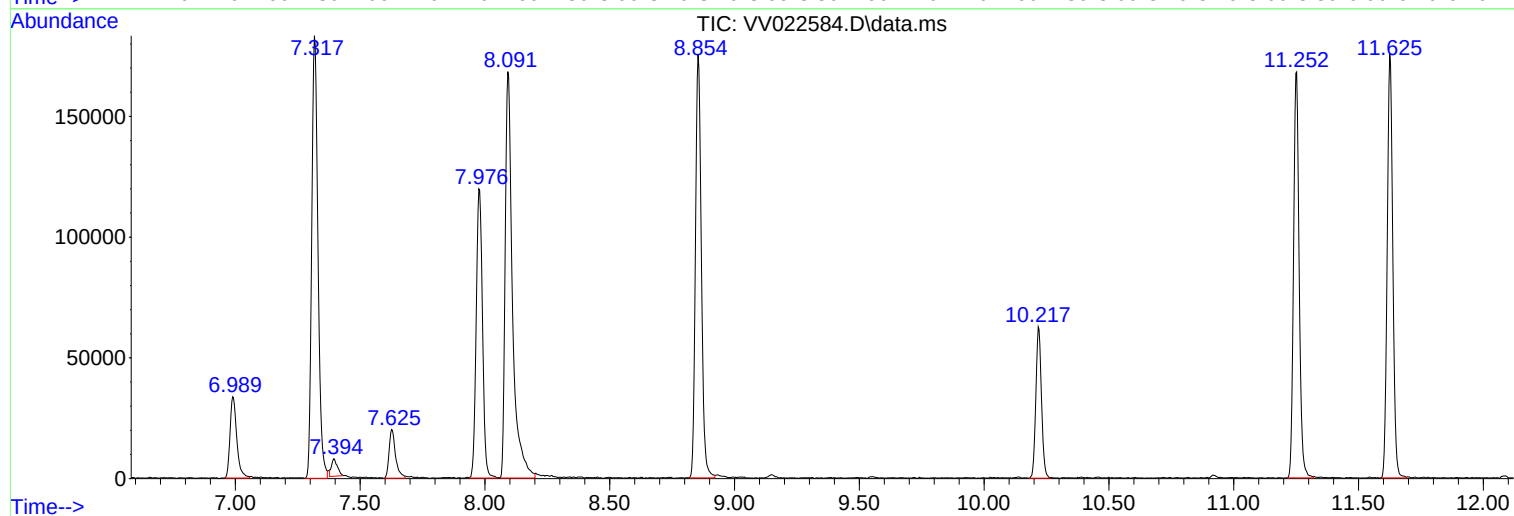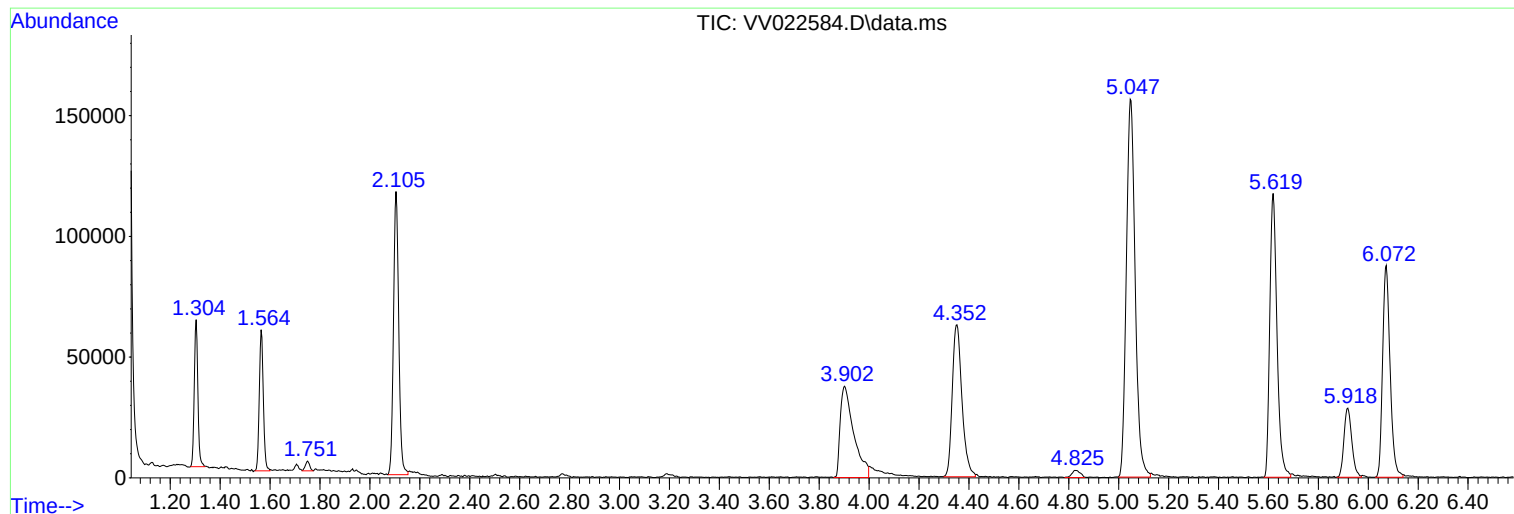

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022581.D
Acq On : 05 Oct 2021 18:39
Operator : SY/MD
Sample : M4052-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022581.D
Acq On : 05 Oct 2021 18:39
Operator : SY/MD
Sample : M4052-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
