

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022586.D
 Acq On : 05 Oct 2021 22:35
 Operator : SY/MD
 Sample : M4051-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rVB	64444	63838	16.47%	2.094%
2	1.565	153	163	173	rBV	59061	65110	16.80%	2.136%
3	2.105	321	331	348	rBV	111061	163727	42.25%	5.370%
4	3.880	873	883	909	rBV2	49426	136737	35.28%	4.485%
5	4.349	1013	1029	1053	rBV2	64195	170228	43.93%	5.584%
6	5.047	1230	1246	1275	rBV2	153854	387523	100.00%	12.711%
7	5.619	1412	1424	1444	rBV	109283	222546	57.43%	7.300%
8	5.912	1504	1515	1530	rBV8	5313	11482	2.96%	0.377%
9	6.072	1551	1565	1585	rBV	89271	179949	46.44%	5.902%
10	6.989	1839	1850	1868	rBV	33451	60875	15.71%	1.997%
11	7.317	1941	1952	1970	rBV	184321	317294	81.88%	10.407%
12	7.394	1971	1976	1991	rVB3	4761	8528	2.20%	0.280%
13	7.625	2036	2048	2063	rBV	19385	34483	8.90%	1.131%
14	8.092	2182	2193	2233	rBV2	166856	337087	86.99%	11.057%
15	8.854	2418	2430	2453	rBV	167801	273942	70.69%	8.985%
16	10.217	2844	2854	2871	rBV2	59723	95241	24.58%	3.124%
17	11.249	3163	3175	3193	rBV	156481	243065	62.72%	7.973%
18	11.625	3281	3292	3314	rBV	171755	272767	70.39%	8.947%
19	15.982	4639	4647	4653	rBV8	2481	4324	1.12%	0.142%




Sum of corrected areas: 3048746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022586.D
Acq On : 05 Oct 2021 22:35
Operator : SY/MD
Sample : M4051-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

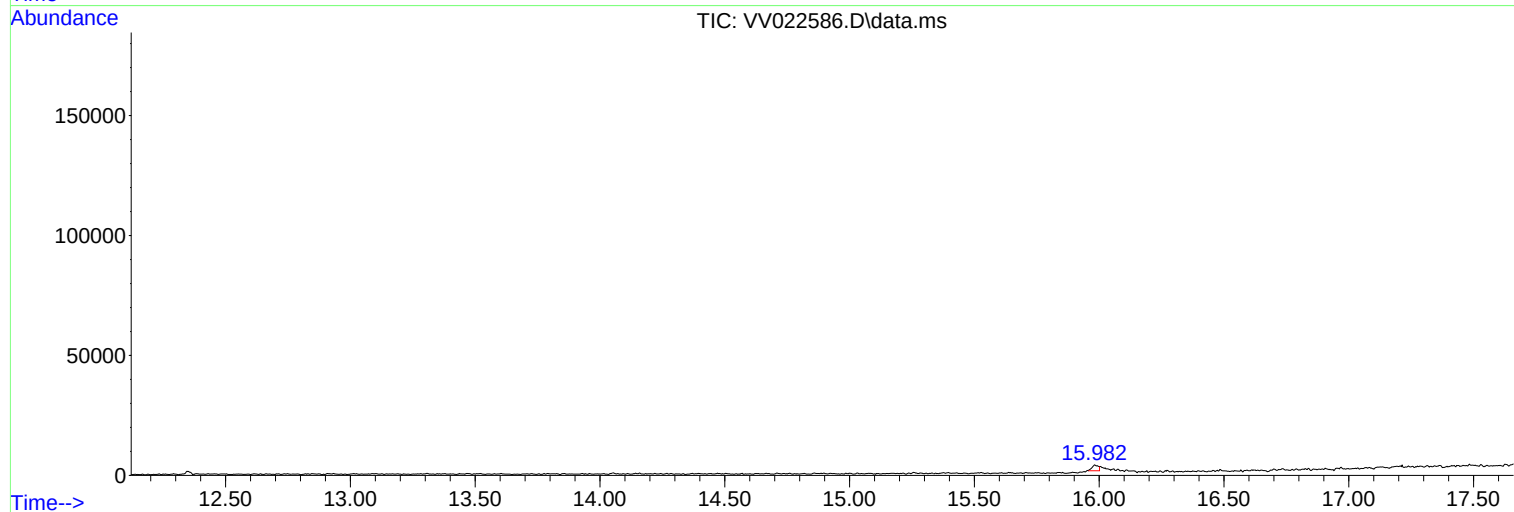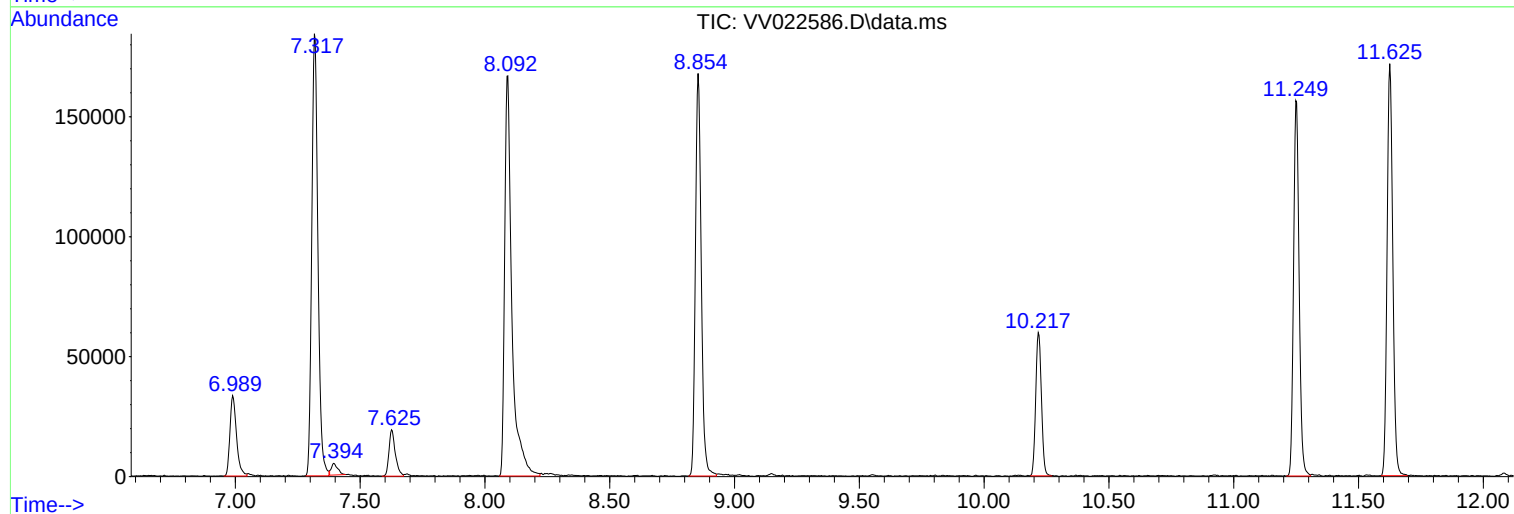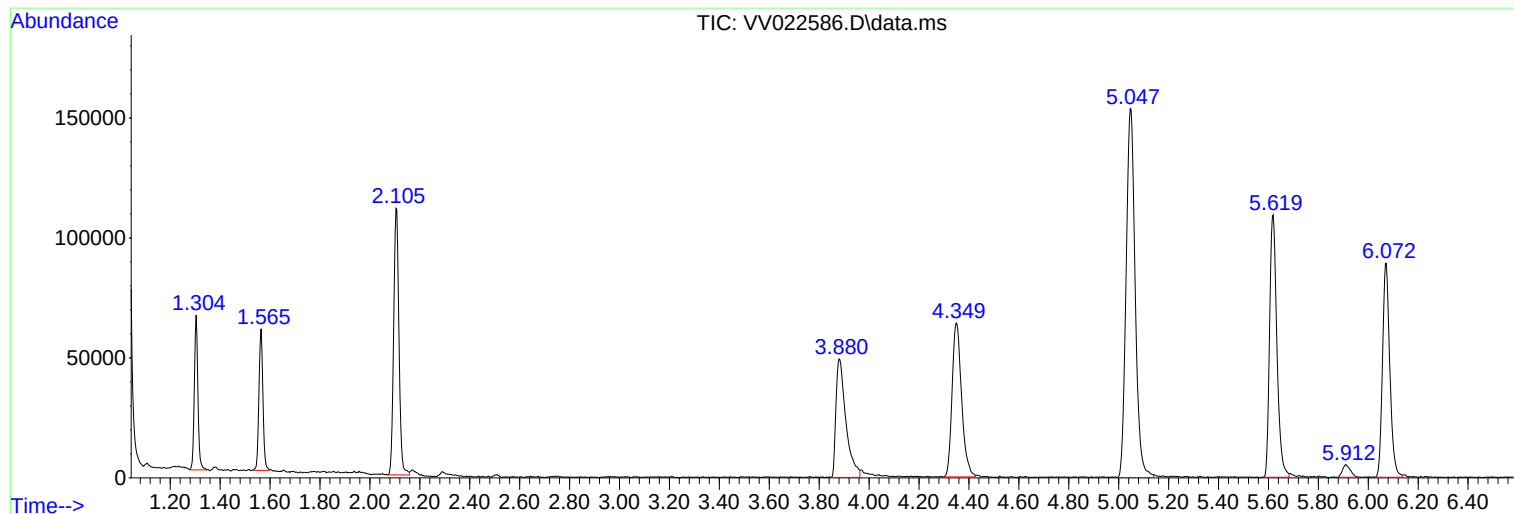

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022586.D
Acq On : 05 Oct 2021 22:35
Operator : SY/MD
Sample : M4051-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022586.D
Acq On : 05 Oct 2021 22:35
Operator : SY/MD
Sample : M4051-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
