

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022587.D
 Acq On : 05 Oct 2021 22:59
 Operator : SY/MD
 Sample : M4051-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	96	rVB	59732	62650	12.76%	1.442%
2	1.565	155	163	177	rVB	54171	63379	12.91%	1.458%
3	1.928	270	276	284	rVB4	5279	7246	1.48%	0.167%
4	2.108	320	332	346	rBV3	193066	324413	66.08%	7.465%
5	3.188	654	668	681	rBV3	4092	8457	1.72%	0.195%
6	3.905	875	891	926	rBV	185213	490925	100.00%	11.297%
7	4.346	1010	1028	1055	rBV	65414	176445	35.94%	4.060%
8	4.825	1168	1177	1193	rVB4	3383	7774	1.58%	0.179%
9	5.043	1229	1245	1280	rBV2	163348	392614	79.97%	9.035%
10	5.616	1407	1423	1450	rBV	112007	227446	46.33%	5.234%
11	5.912	1502	1515	1538	rBV	187909	373551	76.09%	8.596%
12	6.069	1551	1564	1585	rBV	87855	180256	36.72%	4.148%
13	6.989	1839	1850	1871	rBV	33731	62300	12.69%	1.434%
14	7.317	1940	1952	1969	rBV	177759	312057	63.57%	7.181%
15	7.397	1971	1977	1994	rVB2	4635	9181	1.87%	0.211%
16	7.625	2038	2048	2071	rBV	19762	36626	7.46%	0.843%
17	7.976	2145	2157	2179	rBV	224546	377112	76.82%	8.678%
18	8.095	2184	2194	2231	rBV2	156105	348168	70.92%	8.012%
19	8.854	2419	2430	2448	rBV	166565	274883	55.99%	6.326%
20	10.217	2844	2854	2867	rBV2	59982	95157	19.38%	2.190%
21	11.249	3165	3175	3195	rBV	154766	247455	50.41%	5.694%
22	11.625	3278	3292	3308	rBV	169843	267477	54.48%	6.155%




Sum of corrected areas: 4345572

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022587.D
Acq On : 05 Oct 2021 22:59
Operator : SY/MD
Sample : M4051-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

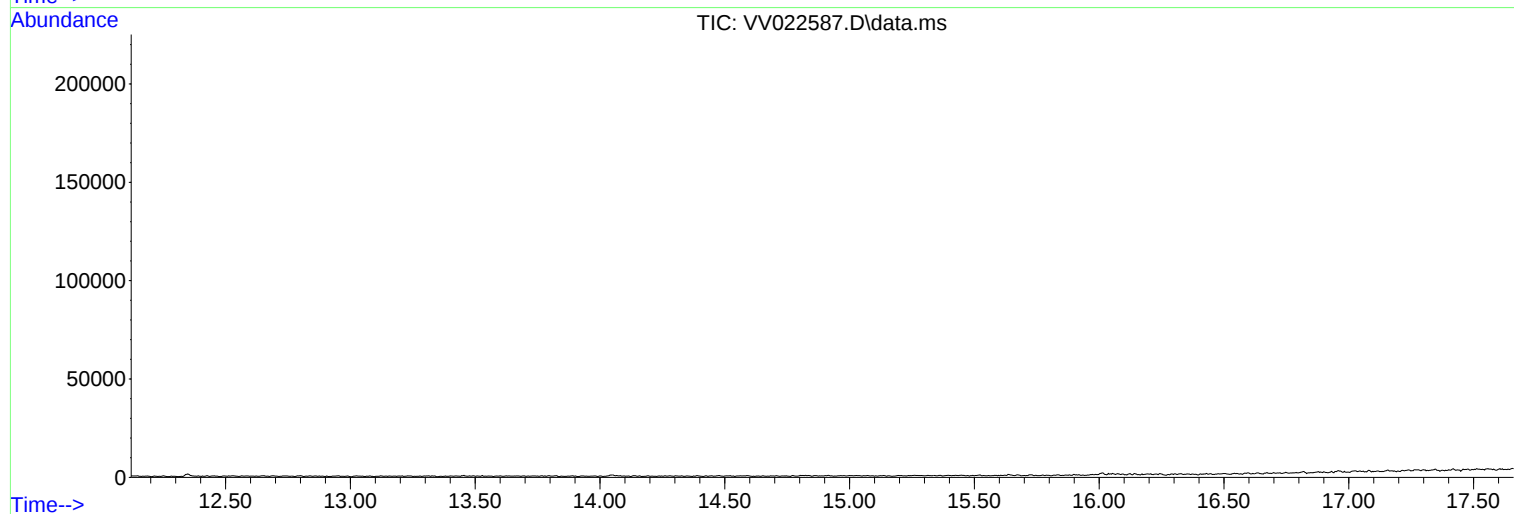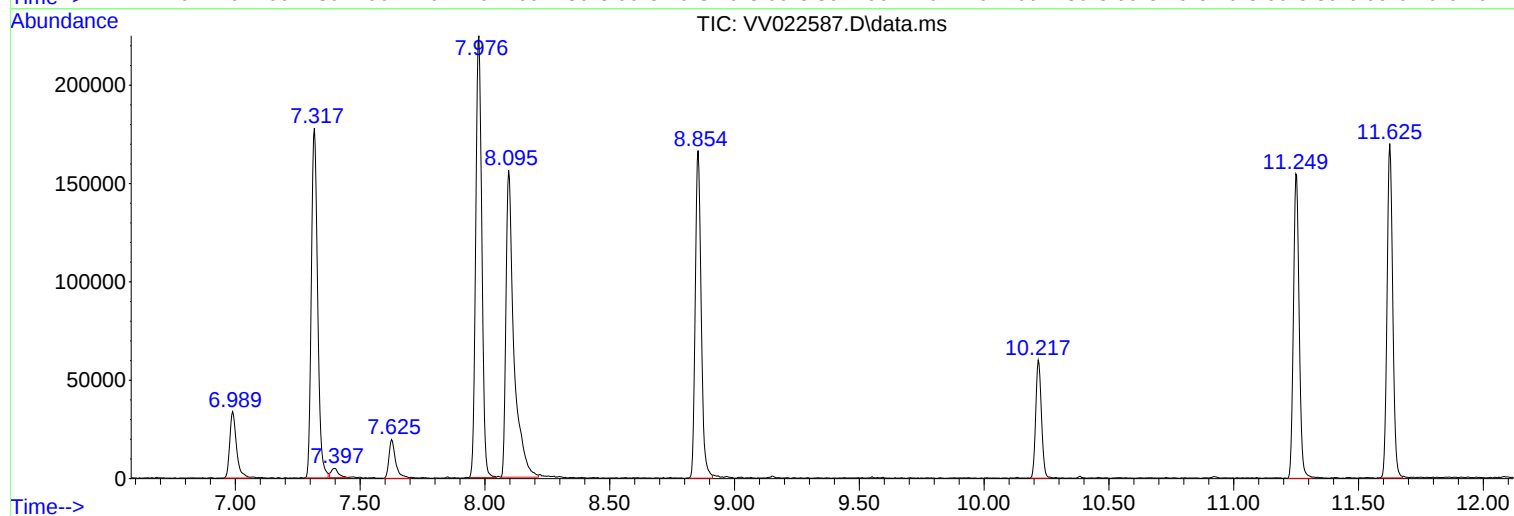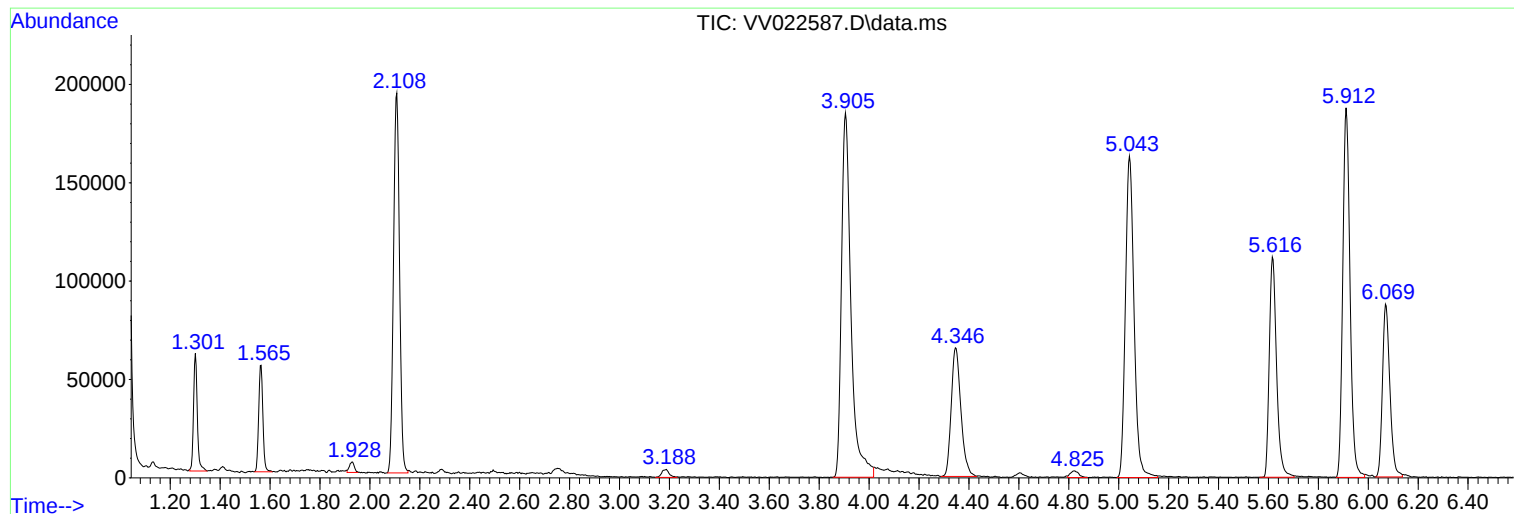

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022587.D
Acq On : 05 Oct 2021 22:59
Operator : SY/MD
Sample : M4051-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022587.D
Acq On : 05 Oct 2021 22:59
Operator : SY/MD
Sample : M4051-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
