

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022588.D
 Acq On : 05 Oct 2021 23:23
 Operator : SY/MD
 Sample : M4051-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	98	rVB	62642	65659	16.45%	2.019%
2	1.564	156	163	175	rBV	57716	64750	16.22%	1.991%
3	2.101	320	330	343	rBV	111459	162394	40.69%	4.993%
4	3.908	881	892	926	rBV2	33967	131536	32.96%	4.045%
5	4.349	1012	1029	1053	rBV	68556	180144	45.14%	5.539%
6	4.825	1161	1177	1188	rBV3	3458	7953	1.99%	0.245%
7	5.047	1230	1246	1273	rBV2	167629	399086	100.00%	12.272%
8	5.616	1411	1423	1449	rBV	116886	239908	60.11%	7.377%
9	5.915	1503	1516	1537	rVB5	14074	33019	8.27%	1.015%
10	6.072	1552	1565	1584	rBV	90523	186308	46.68%	5.729%
11	6.989	1840	1850	1866	rBV2	34401	62125	15.57%	1.910%
12	7.317	1940	1952	1970	rBV	188248	323735	81.12%	9.955%
13	7.391	1970	1975	1992	rVB4	4352	8836	2.21%	0.272%
14	7.625	2039	2048	2068	rBV	21182	38207	9.57%	1.175%
15	7.979	2141	2158	2169	rBV4	22405	40169	10.07%	1.235%
16	8.095	2184	2194	2235	rBV3	161060	367333	92.04%	11.295%
17	8.854	2419	2430	2454	rBV	182220	297324	74.50%	9.142%
18	10.217	2845	2854	2868	rBV	61739	98695	24.73%	3.035%
19	11.249	3164	3175	3196	rBV	166922	261656	65.56%	8.046%
20	11.625	3279	3292	3311	rBV	176068	278923	69.89%	8.577%
21	12.349	3510	3517	3523	rBV5	3591	4350	1.09%	0.134%




Sum of corrected areas: 3252110

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022588.D
Acq On : 05 Oct 2021 23:23
Operator : SY/MD
Sample : M4051-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

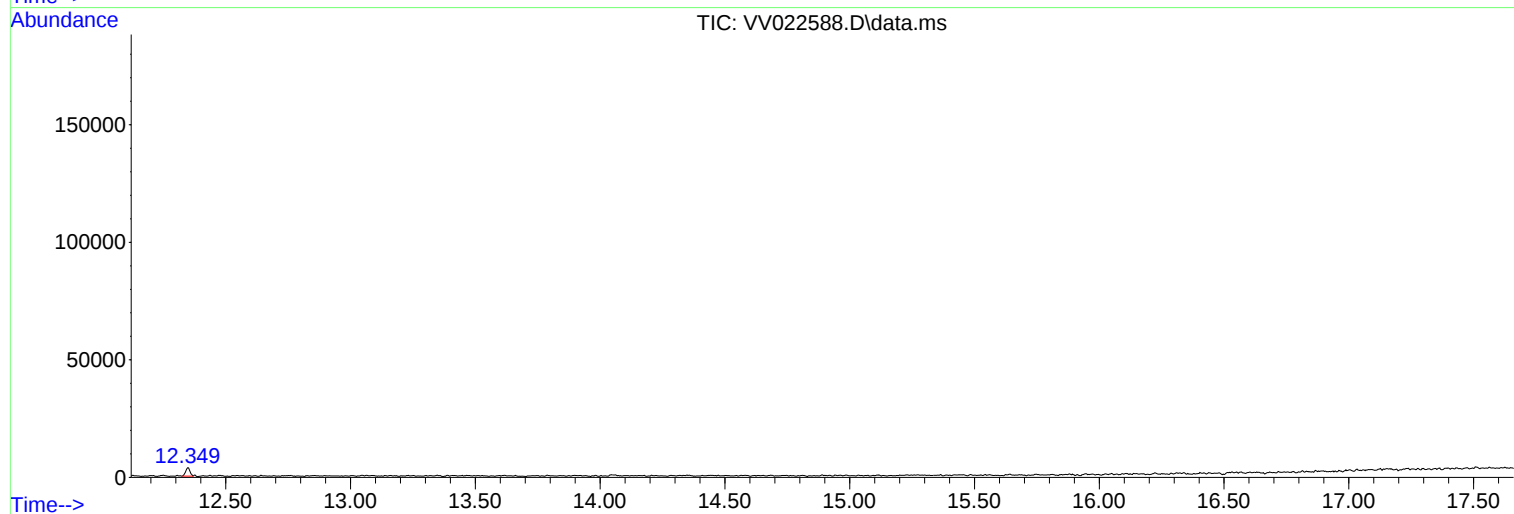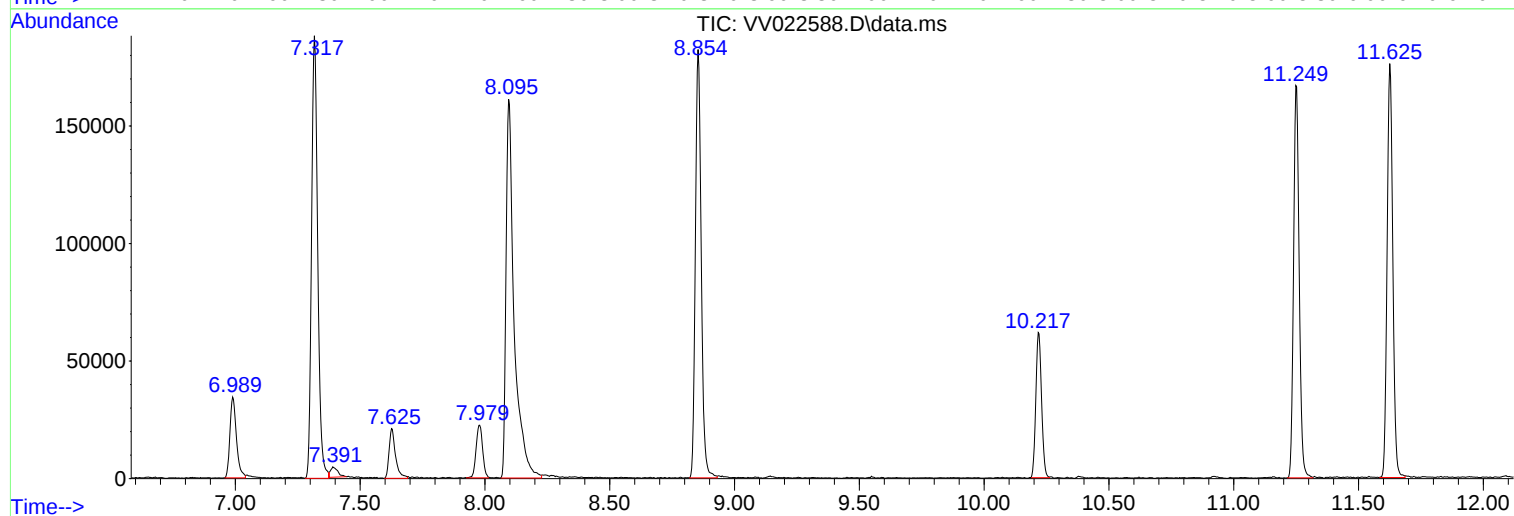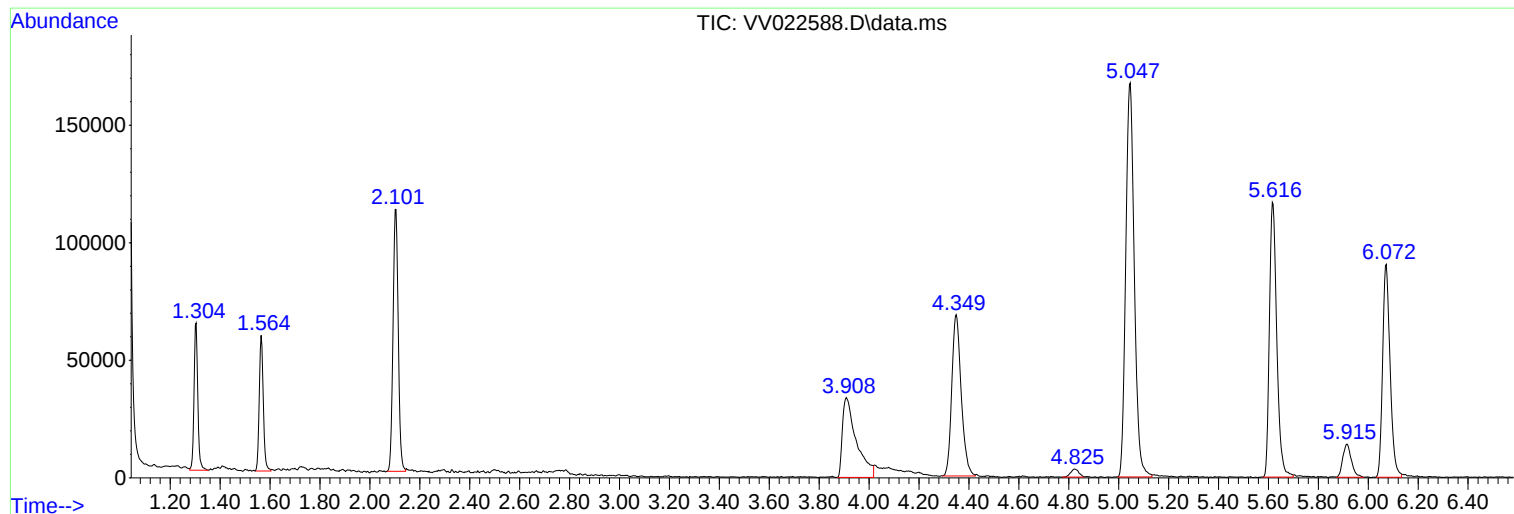

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022588.D
Acq On : 05 Oct 2021 23:23
Operator : SY/MD
Sample : M4051-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022588.D
Acq On : 05 Oct 2021 23:23
Operator : SY/MD
Sample : M4051-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------