

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022589.D
 Acq On : 05 Oct 2021 23:48
 Operator : SY/MD
 Sample : M4051-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	59095	59189	15.48%	1.954%
2	1.564	155	163	176	rBV	54547	62079	16.24%	2.049%
3	2.105	319	331	345	rBV	107081	153485	40.15%	5.066%
4	3.915	883	894	923	rBV2	30353	121364	31.75%	4.006%
5	4.349	1011	1029	1055	rVB	66194	170012	44.48%	5.612%
6	5.043	1230	1245	1273	rBV3	162226	382239	100.00%	12.617%
7	5.616	1411	1423	1449	rBV	114482	230363	60.27%	7.604%
8	5.912	1502	1515	1530	rBV	5543	13017	3.41%	0.430%
9	6.072	1552	1565	1588	rBV2	86933	178659	46.74%	5.897%
10	6.989	1841	1850	1876	rBV	31862	62069	16.24%	2.049%
11	7.317	1940	1952	1968	rBV	174889	306477	80.18%	10.117%
12	7.397	1972	1977	1984	rVB4	3414	5277	1.38%	0.174%
13	7.625	2039	2048	2066	rBV2	19592	35056	9.17%	1.157%
14	7.979	2150	2158	2170	rVB4	4523	7345	1.92%	0.242%
15	8.098	2184	2195	2233	rBV2	150349	347959	91.03%	11.486%
16	8.854	2413	2430	2455	rBV	171296	284219	74.36%	9.382%
17	10.220	2842	2855	2872	rVB	61112	96951	25.36%	3.200%
18	11.249	3164	3175	3192	rBV	161707	252131	65.96%	8.323%
19	11.625	3280	3292	3306	rBV	166404	261576	68.43%	8.634%




Sum of corrected areas: 3029467

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022589.D
Acq On : 05 Oct 2021 23:48
Operator : SY/MD
Sample : M4051-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

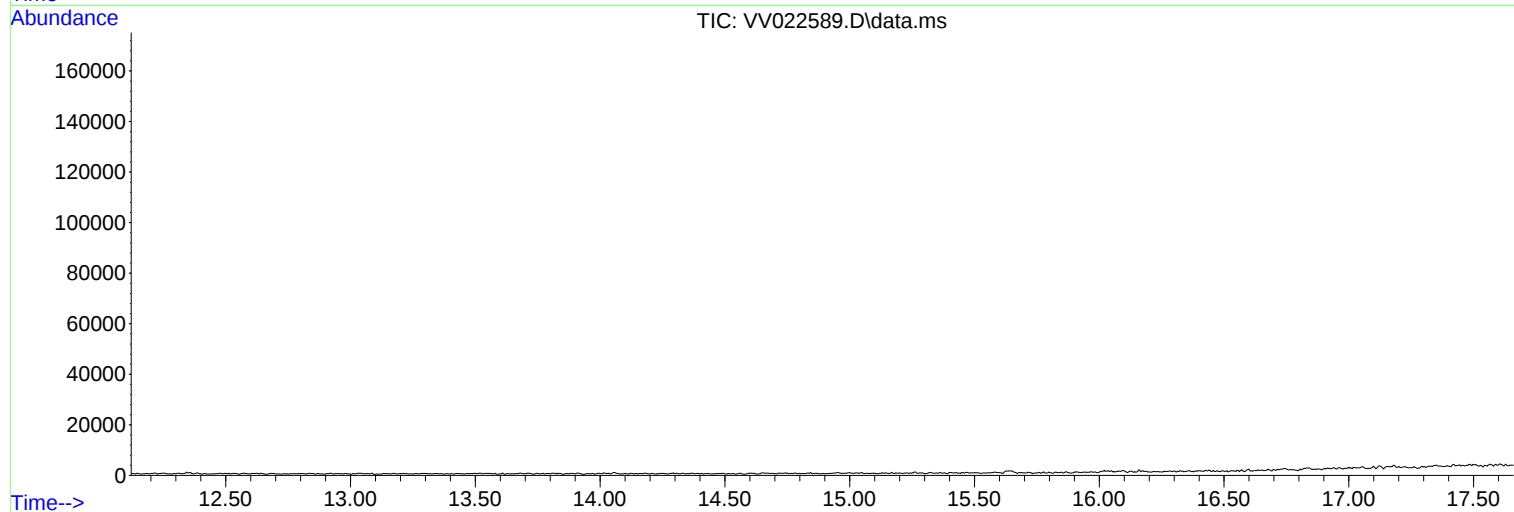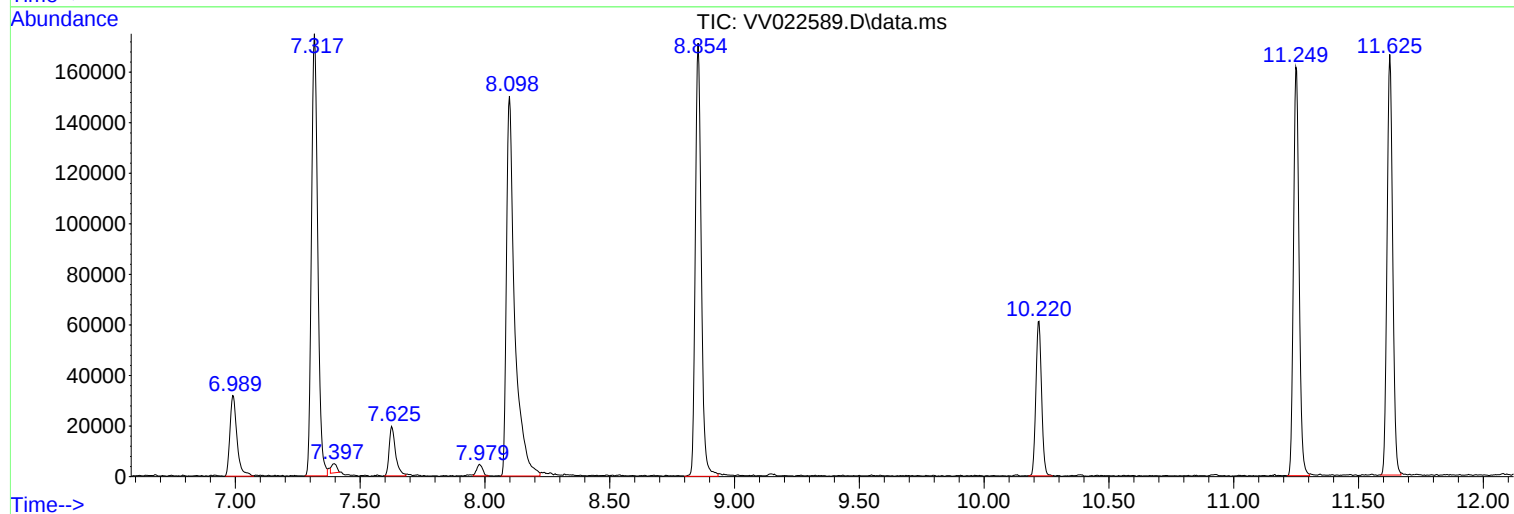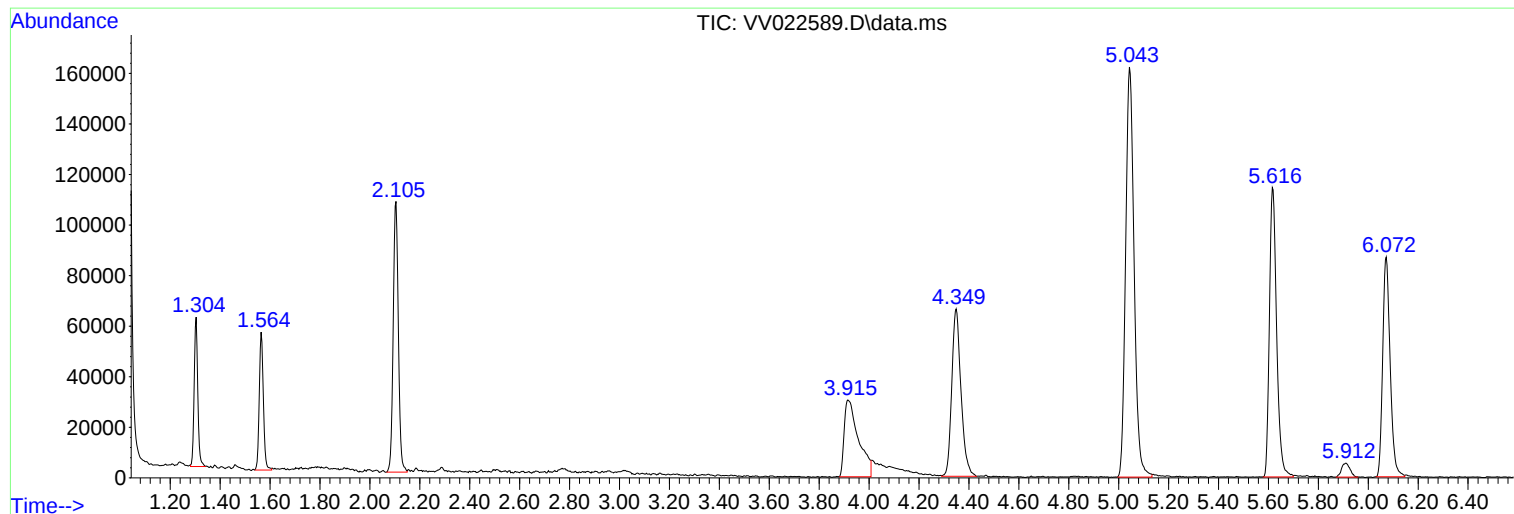

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022589.D
Acq On : 05 Oct 2021 23:48
Operator : SY/MD
Sample : M4051-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022589.D
Acq On : 05 Oct 2021 23:48
Operator : SY/MD
Sample : M4051-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
