

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022590.D
 Acq On : 06 Oct 2021 00:12
 Operator : SY/MD
 Sample : M4051-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	93	rVB2	63477	76716	19.64%	2.375%
2	1.564	155	163	173	rBV	58114	62622	16.03%	1.939%
3	2.105	321	331	346	rBV	110853	163716	41.91%	5.069%
4	2.169	346	351	370	rVB3	3714	7621	1.95%	0.236%
5	2.291	380	389	401	rBV	21180	31470	8.06%	0.974%
6	3.883	873	884	915	rBV	55643	162675	41.64%	5.037%
7	4.349	1012	1029	1055	rBV	68121	178065	45.58%	5.514%
8	5.047	1230	1246	1278	rBV3	155020	389410	99.68%	12.058%
9	5.619	1411	1424	1449	rBV	108664	222275	56.90%	6.883%
10	5.908	1504	1514	1531	rVB7	9003	19416	4.97%	0.601%
11	6.072	1552	1565	1586	rBV	88002	182077	46.61%	5.638%
12	6.989	1839	1850	1869	rBV2	33920	63882	16.35%	1.978%
13	7.317	1939	1952	1970	rBV	181096	317850	81.36%	9.842%
14	7.625	2038	2048	2065	rBV2	20134	36014	9.22%	1.115%
15	8.092	2181	2193	2225	rBV2	182987	390664	100.00%	12.097%
16	8.854	2417	2430	2453	rBV	168049	280719	71.86%	8.692%
17	10.217	2842	2854	2873	rBV2	59874	94234	24.12%	2.918%
18	11.249	3163	3175	3191	rBV	161668	251592	64.40%	7.790%
19	11.625	3280	3292	3308	rBV	179690	279925	71.65%	8.668%
20	16.564	4818	4828	4837	rBV2	12357	18582	4.76%	0.575%




Sum of corrected areas: 3229525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022590.D
Acq On : 06 Oct 2021 00:12
Operator : SY/MD
Sample : M4051-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

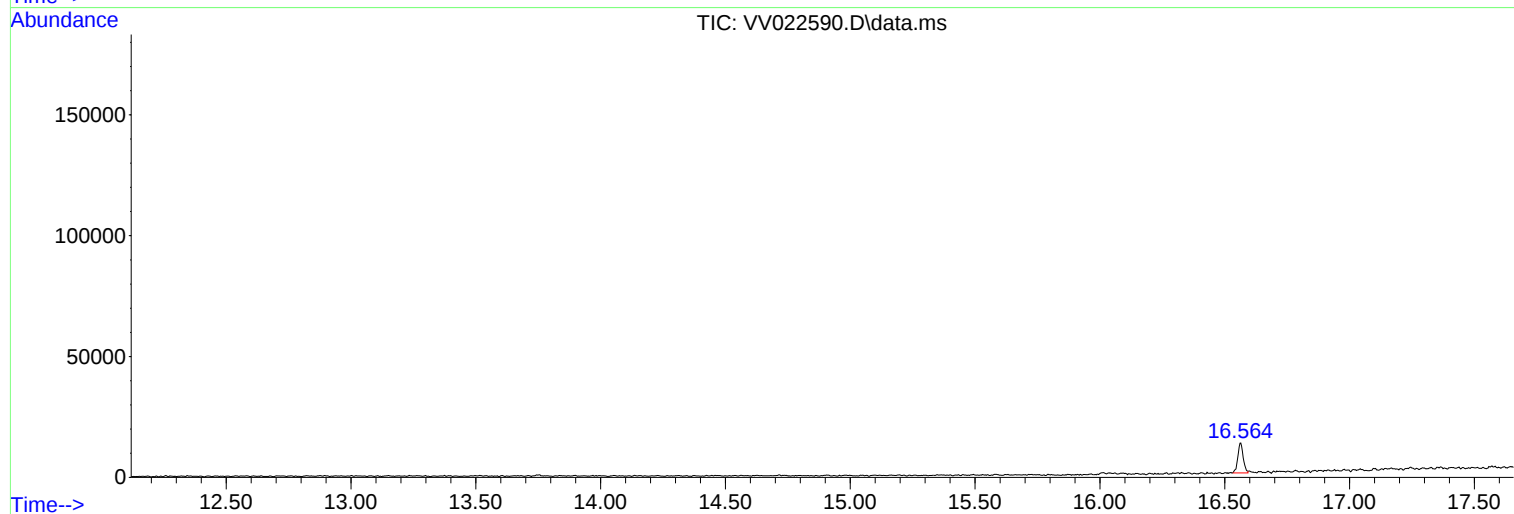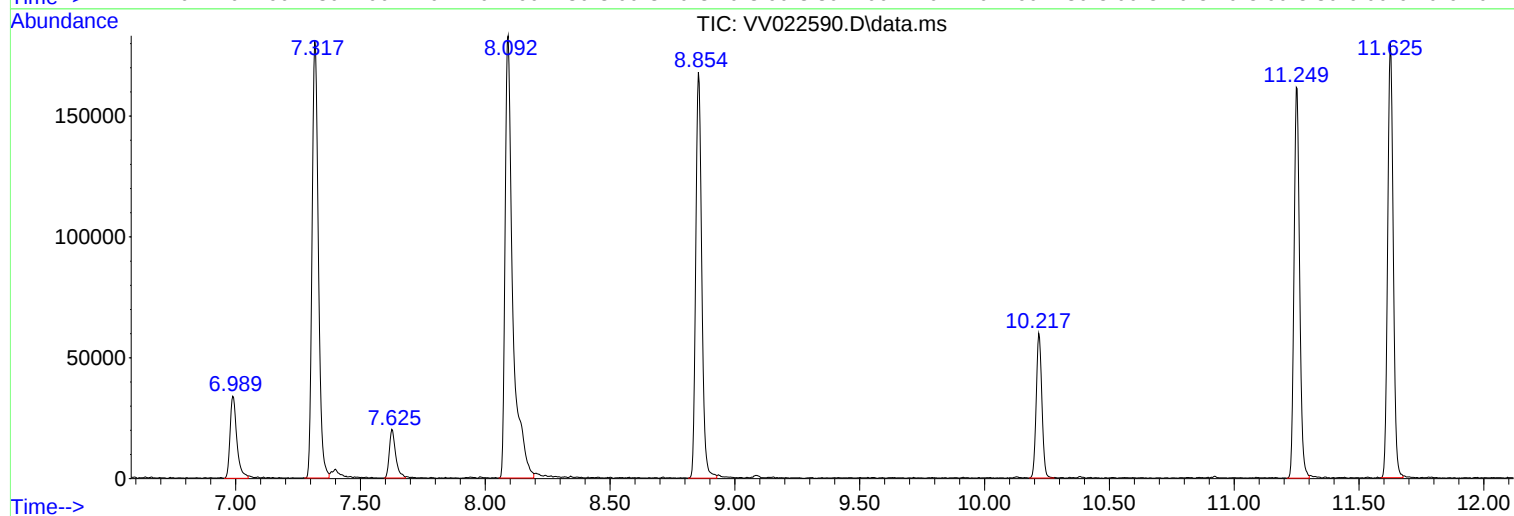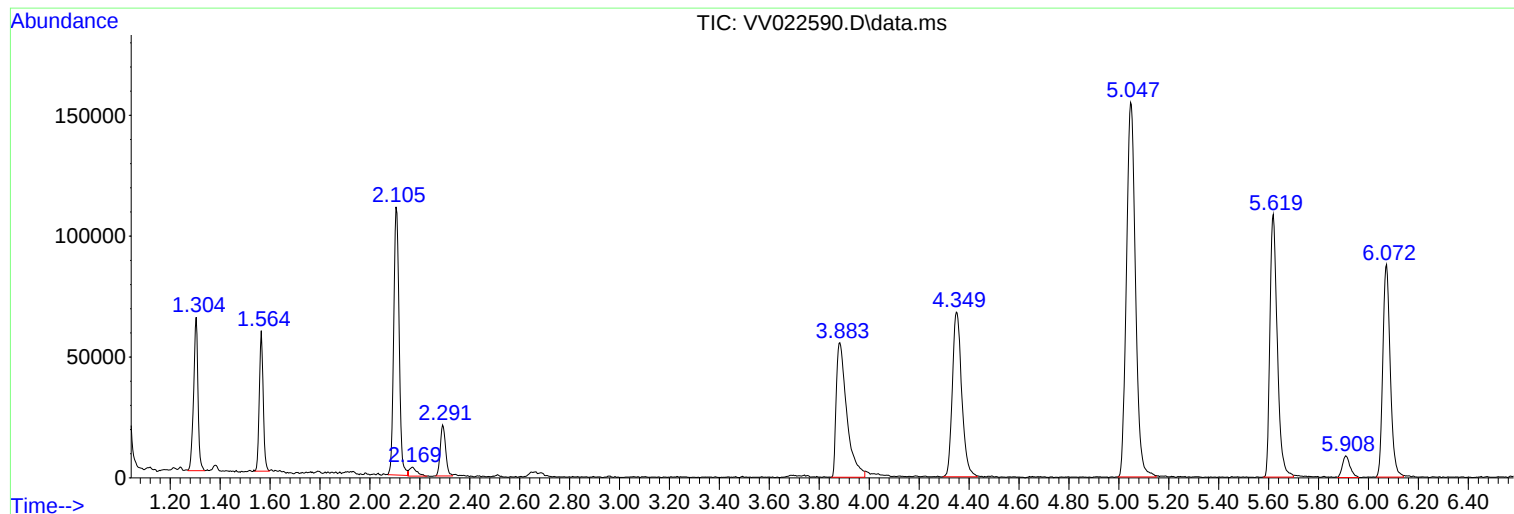

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022590.D
Acq On : 06 Oct 2021 00:12
Operator : SY/MD
Sample : M4051-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022590.D
Acq On : 06 Oct 2021 00:12
Operator : SY/MD
Sample : M4051-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
