

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022593.D
 Acq On : 06 Oct 2021 01:24
 Operator : SY/MD
 Sample : M4051-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	64536	66533	16.36%	1.881%
2	1.526	145	151	156	rBV	14105	14481	3.56%	0.409%
3	1.564	156	163	175	rVB	56681	65411	16.08%	1.849%
4	1.934	268	278	288	rVB	45672	63953	15.72%	1.808%
5	2.108	321	332	348	rBV	115270	169723	41.73%	4.798%
6	3.883	873	884	917	rBV	62240	202597	49.81%	5.727%
7	4.349	1014	1029	1058	rBV	69656	179718	44.19%	5.080%
8	5.047	1230	1246	1282	rBV2	161001	405388	99.67%	11.460%
9	5.619	1412	1424	1444	rBV	110150	227499	55.93%	6.431%
10	5.918	1503	1517	1535	rBV3	65260	135050	33.20%	3.818%
11	6.069	1551	1564	1588	rBV	91093	188159	46.26%	5.319%
12	6.989	1839	1850	1867	rBV2	36032	65359	16.07%	1.848%
13	7.317	1939	1952	1971	rBV	189426	329554	81.03%	9.316%
14	7.397	1971	1977	1986	rVB5	4235	7507	1.85%	0.212%
15	7.625	2039	2048	2064	rBV2	21567	37760	9.28%	1.067%
16	7.982	2150	2159	2167	rVB6	3967	6531	1.61%	0.185%
17	8.088	2182	2192	2233	rBV2	204323	406721	100.00%	11.498%
18	8.854	2419	2430	2454	rBV	173137	284984	70.07%	8.056%
19	10.217	2838	2854	2867	rBV	67565	107108	26.33%	3.028%
20	11.252	3165	3176	3195	rBV	165744	256940	63.17%	7.263%
21	11.625	3278	3292	3310	rBV	183374	290913	71.53%	8.224%
22	16.564	4818	4828	4839	rBV	16315	25572	6.29%	0.723%




Sum of corrected areas: 3537461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022593.D
Acq On : 06 Oct 2021 01:24
Operator : SY/MD
Sample : M4051-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

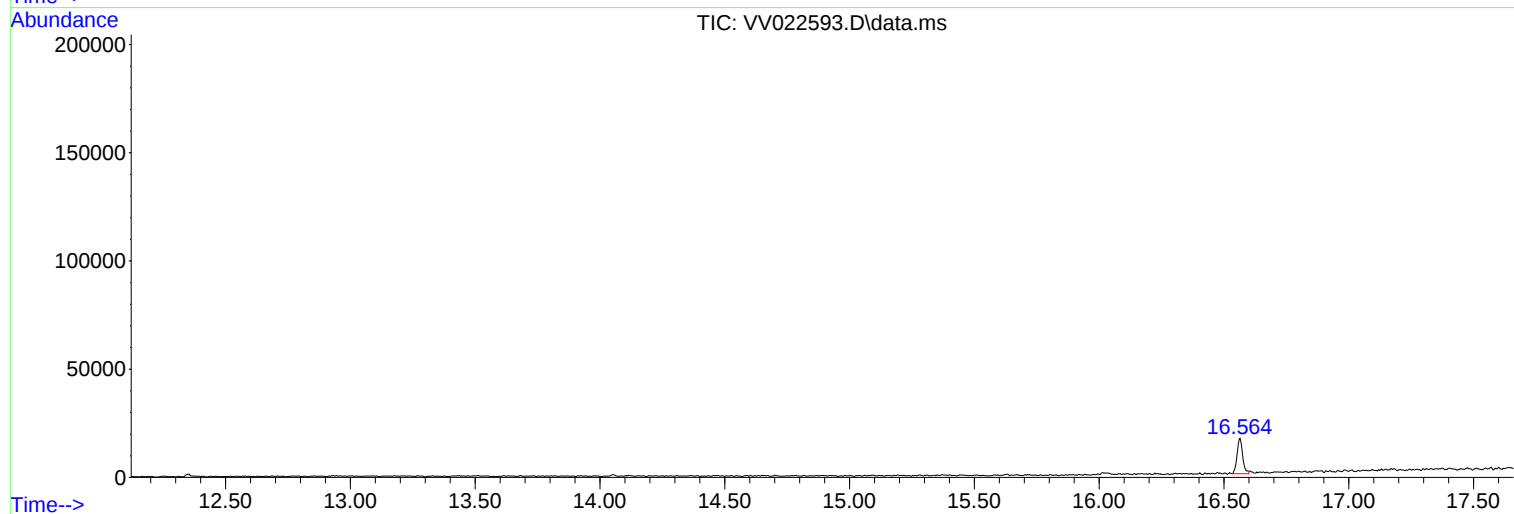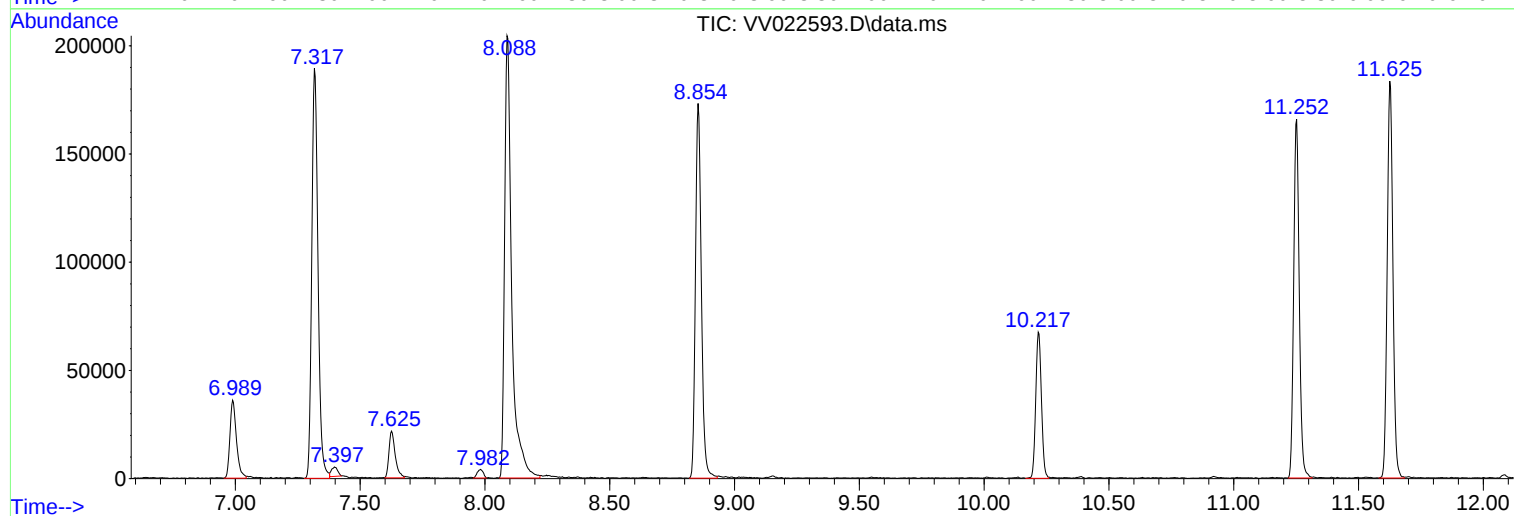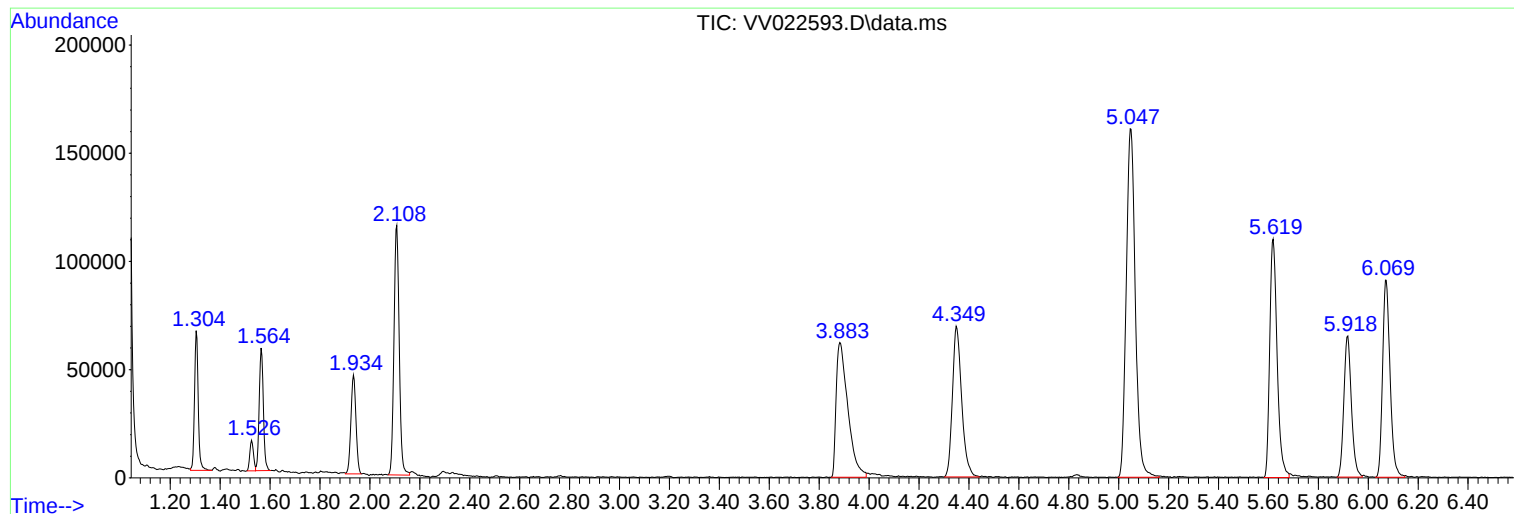

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022593.D
Acq On : 06 Oct 2021 01:24
Operator : SY/MD
Sample : M4051-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1,1-Dichloro-1-fluoroethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.934	1.41 ug/L	63953	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,1-Dichloro-1-fluoroethane	116	C2H3Cl2F	001717-00-6	90
2			1,1-Dichloro-1-fluoroethane	116	C2H3Cl2F	001717-00-6	64
3			Silane, difluorodimethyl-	96	C2H6F2Si	000353-66-2	23
4			1-Chloro-4-methylcyclohexane	132	C7H13Cl	000931-68-0	9
5			Ethanone, 1-(1-methyl-2-cyclopen...	124	C8H12O	068752-16-9	4

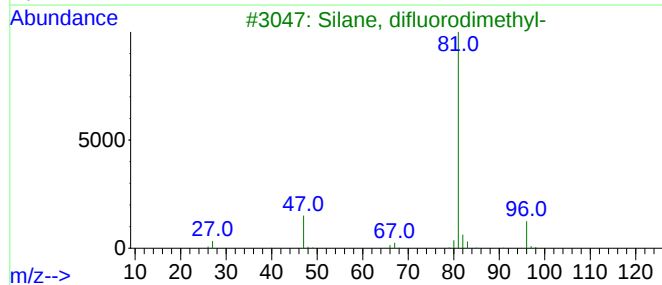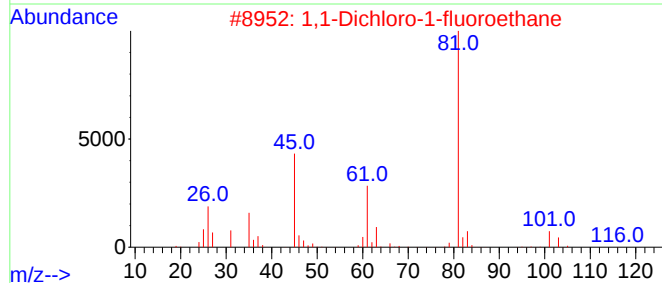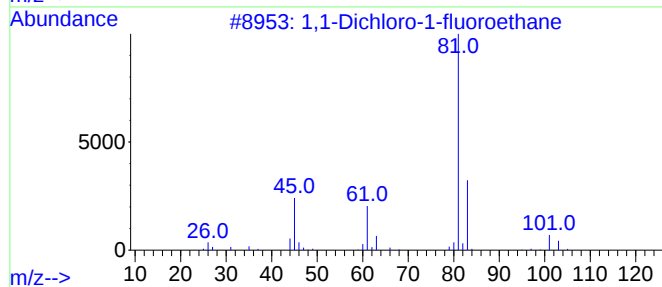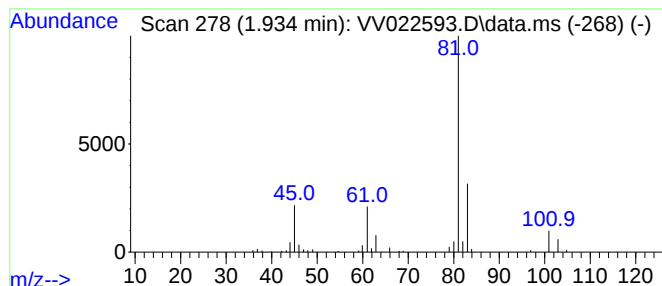

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022593.D
Acq On : 06 Oct 2021 01:24
Operator : SY/MD
Sample : M4051-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,1-Dichloro-1-...	1.934	1.4	ug/L	63953	1	5.619	227499	5.0