

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022596.D
 Acq On : 06 Oct 2021 02:37
 Operator : SY/MD
 Sample : M4050-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7B7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	15	20	26	rBV	22025	18893	4.90%	0.687%
2	1.175	38	42	47	rVB	6201	5249	1.36%	0.191%
3	1.304	74	82	96	rVB2	32783	39251	10.18%	1.428%
4	1.564	155	163	175	rVB	39884	45286	11.74%	1.647%
5	2.104	321	331	344	rBV	60990	91007	23.60%	3.311%
6	2.169	345	351	361	rVB2	4377	7675	1.99%	0.279%
7	2.294	380	390	399	rBV	4479	6578	1.71%	0.239%
8	3.879	868	883	912	rBV	57382	158260	41.04%	5.757%
9	4.352	1014	1030	1054	rBV2	53106	136432	35.38%	4.963%
10	5.047	1231	1246	1279	rBV2	113674	288467	74.81%	10.494%
11	5.619	1412	1424	1452	rBV	113550	230991	59.90%	8.403%
12	5.911	1505	1515	1530	rVB8	5058	10652	2.76%	0.388%
13	6.072	1553	1565	1589	rBV	71325	147019	38.13%	5.348%
14	6.992	1840	1851	1873	rBV3	23620	45099	11.70%	1.641%
15	7.320	1941	1953	1971	rBV	115243	200271	51.94%	7.286%
16	7.628	2039	2049	2069	rBV	14326	25573	6.63%	0.930%
17	8.091	2183	2193	2232	rBV2	192184	385610	100.00%	14.028%
18	8.249	2236	2242	2255	rVB5	3931	6860	1.78%	0.250%
19	8.853	2418	2430	2448	rBV	175974	287341	74.52%	10.453%
20	9.818	2721	2730	2738	rBV4	2773	4007	1.04%	0.146%
21	10.220	2844	2855	2869	rBV	58663	92628	24.02%	3.370%
22	11.152	3138	3145	3154	rBV5	5758	8122	2.11%	0.295%
23	11.252	3165	3176	3196	rBV	171333	266322	69.07%	9.689%
24	11.532	3257	3263	3271	rBV5	3302	5179	1.34%	0.188%
25	11.625	3281	3292	3313	rBV	131435	209816	54.41%	7.633%
26	12.345	3506	3516	3527	rBV4	11853	17385	4.51%	0.632%
27	16.561	4821	4827	4838	rBV3	5313	8841	2.29%	0.322%




Sum of corrected areas: 2748814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022596.D
Acq On : 06 Oct 2021 02:37
Operator : SY/MD
Sample : M4050-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

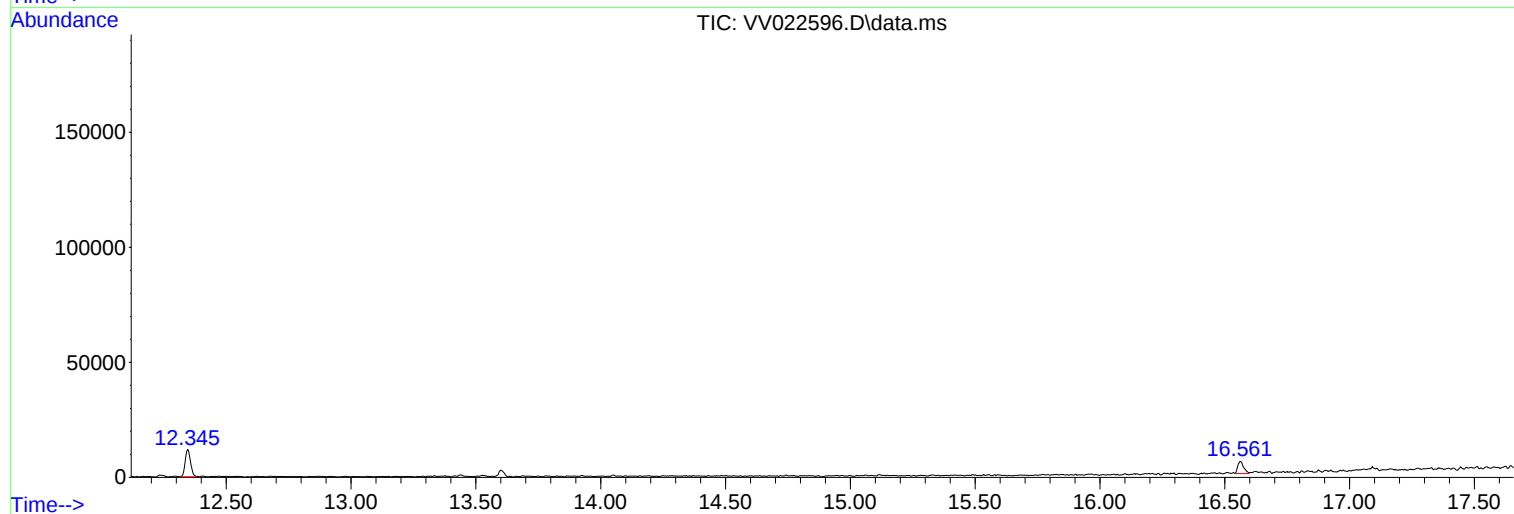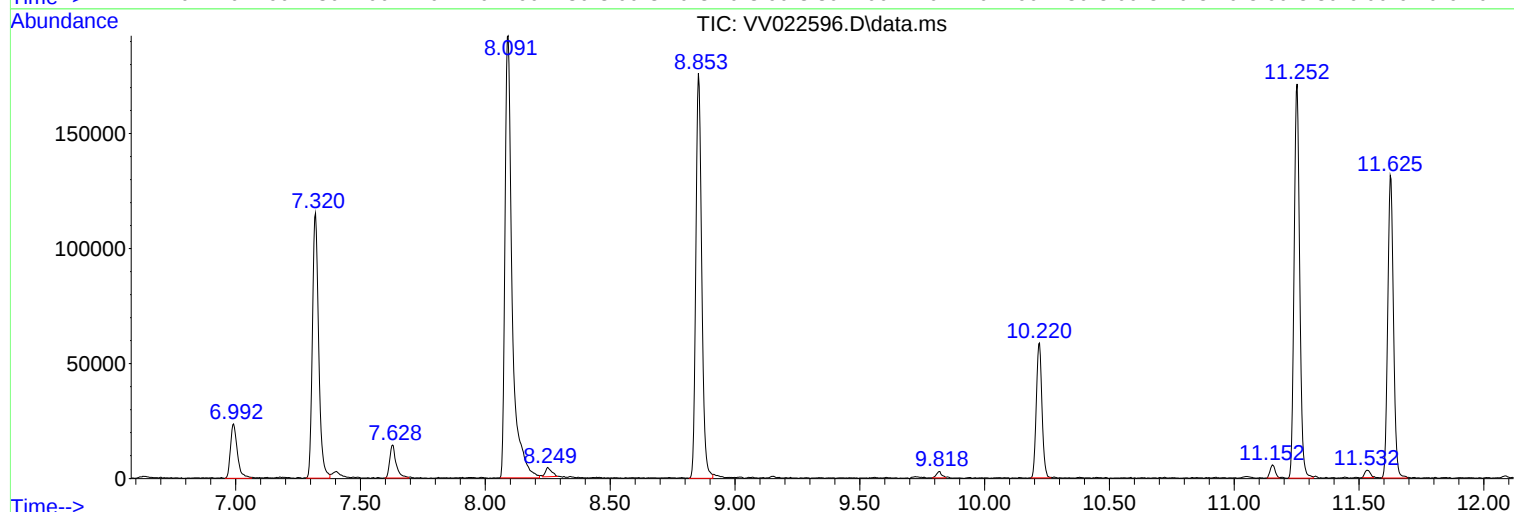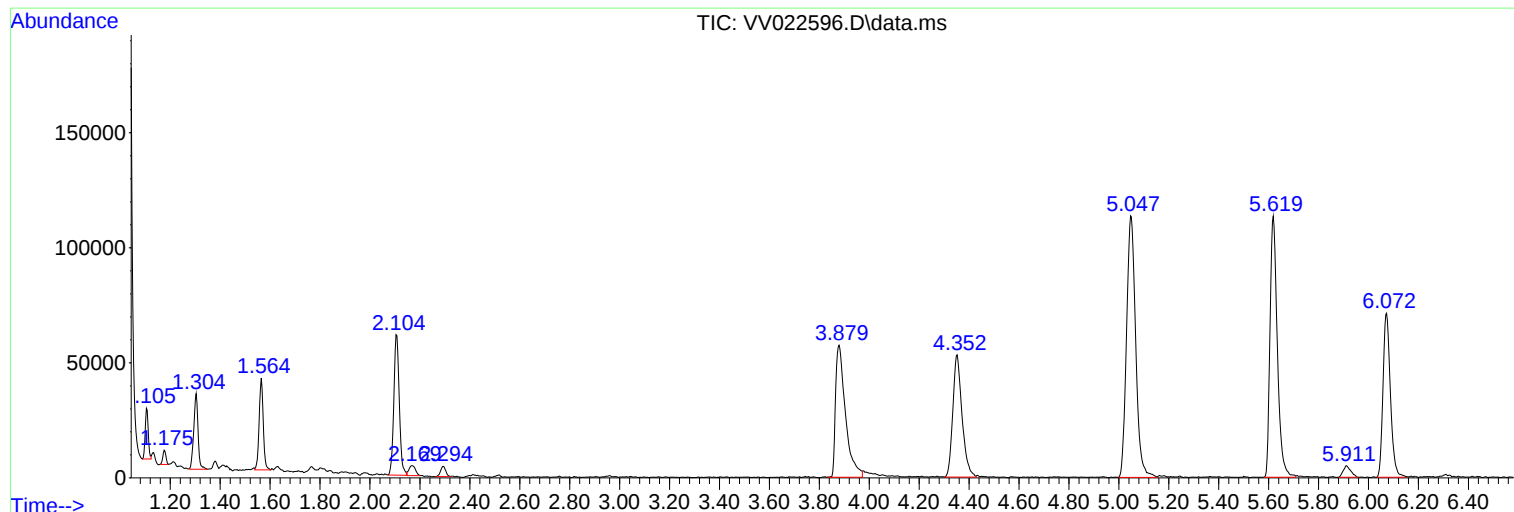

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022596.D
Acq On : 06 Oct 2021 02:37
Operator : SY/MD
Sample : M4050-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022596.D
Acq On : 06 Oct 2021 02:37
Operator : SY/MD
Sample : M4050-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7B7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
