

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022602.D
 Acq On : 06 Oct 2021 05:02
 Operator : SY/MD
 Sample : M4050-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	25	29	35	rVB2	4809	4630	1.10%	0.167%
2	1.301	76	81	92	rVB	27449	29399	6.98%	1.061%
3	1.565	155	163	176	rBV	39569	45830	10.88%	1.654%
4	2.105	316	331	342	rBV	63104	91660	21.76%	3.308%
5	3.905	880	891	933	rBV	36124	165968	39.40%	5.990%
6	4.349	1012	1029	1051	rBV2	54762	141830	33.67%	5.119%
7	5.050	1231	1247	1267	rBV2	120659	301204	71.50%	10.871%
8	5.619	1412	1424	1442	rBV	111109	225838	53.61%	8.151%
9	5.912	1504	1515	1529	rBV6	5287	11717	2.78%	0.423%
10	6.072	1551	1565	1584	rBV	74718	153228	36.37%	5.530%
11	6.992	1838	1851	1871	rBV2	24331	46834	11.12%	1.690%
12	7.320	1940	1953	1972	rBV	119782	214226	50.85%	7.732%
13	7.629	2040	2049	2071	rBV2	13915	25348	6.02%	0.915%
14	8.095	2182	2194	2236	rBV2	201532	421251	100.00%	15.204%
15	8.854	2419	2430	2451	rBV	171685	282936	67.17%	10.212%
16	10.217	2842	2854	2874	rVB	64393	101021	23.98%	3.646%
17	11.249	3164	3175	3198	rBV	164001	258211	61.30%	9.319%
18	11.535	3257	3264	3274	rBV5	3252	5149	1.22%	0.186%
19	11.625	3281	3292	3308	rBV	143824	221580	52.60%	7.997%
20	12.345	3508	3516	3527	rBV4	15291	22871	5.43%	0.825%




Sum of corrected areas: 2770731

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022602.D
Acq On : 06 Oct 2021 05:02
Operator : SY/MD
Sample : M4050-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

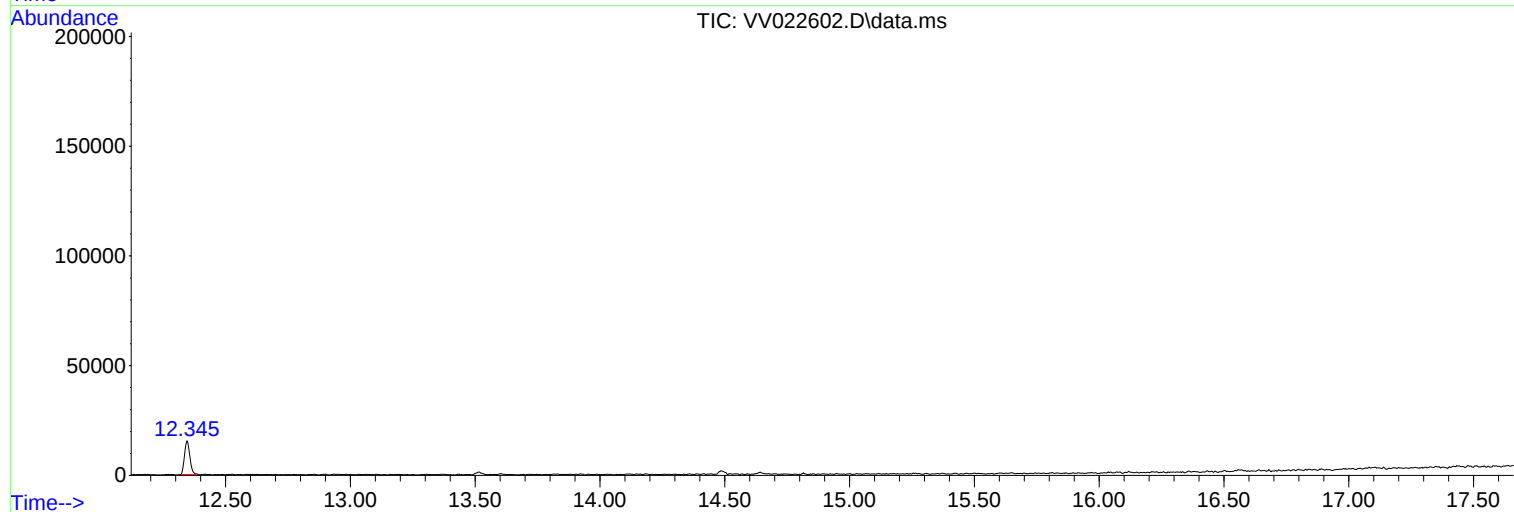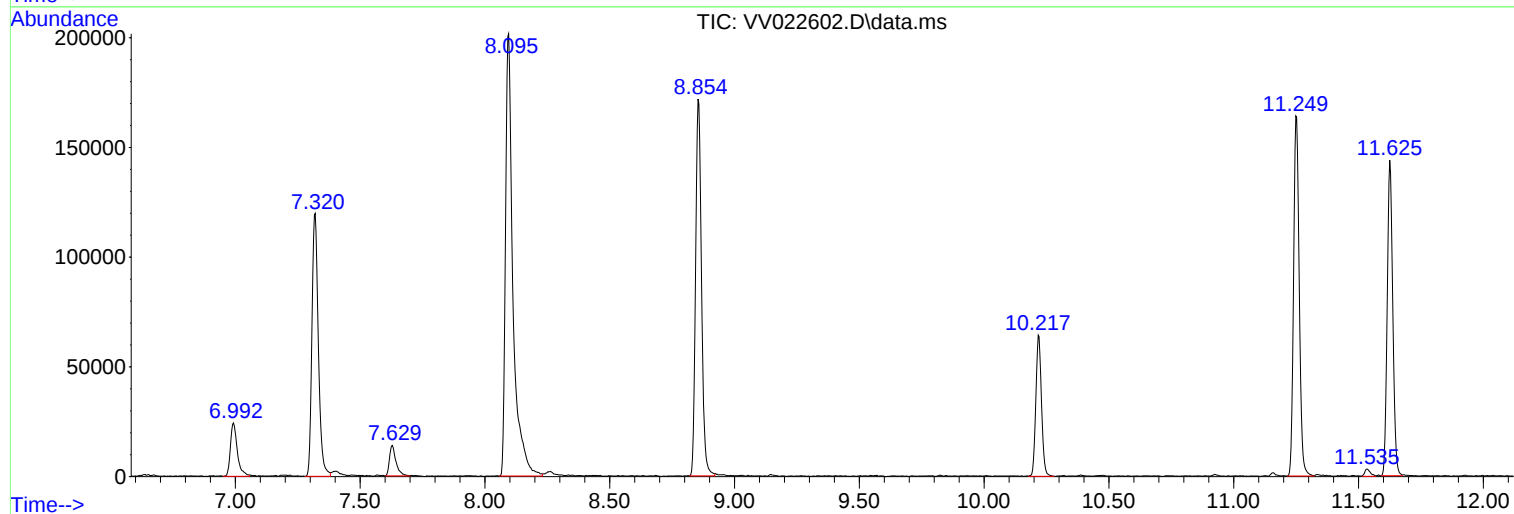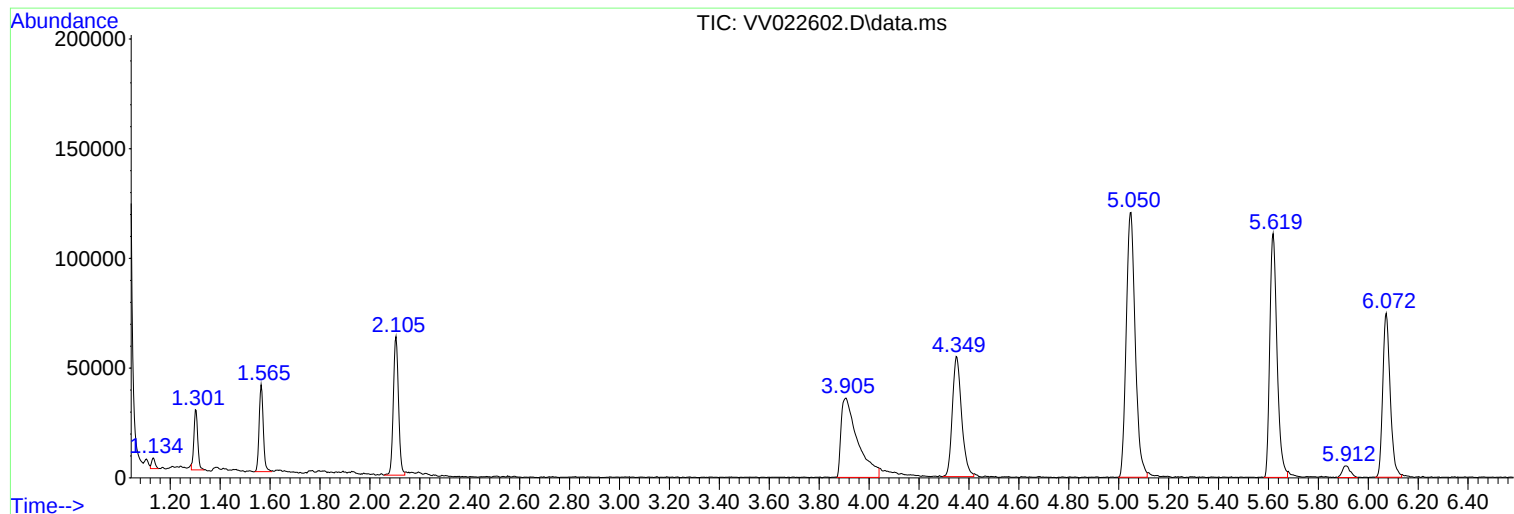

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022602.D
Acq On : 06 Oct 2021 05:02
Operator : SY/MD
Sample : M4050-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022602.D
Acq On : 06 Oct 2021 05:02
Operator : SY/MD
Sample : M4050-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
