

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022605.D
 Acq On : 06 Oct 2021 06:14
 Operator : SY/MD
 Sample : M4050-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7C6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	15	20	25	rVB4	9021	8762	2.21%	0.312%
2	1.134	25	29	38	rVB2	5526	5934	1.50%	0.211%
3	1.304	75	82	93	rVB	29107	31447	7.93%	1.120%
4	1.565	156	163	174	rVB	39391	43458	10.96%	1.548%
5	2.105	321	331	343	rBV	60443	87926	22.18%	3.133%
6	2.172	343	352	374	rVB2	17247	36104	9.11%	1.286%
7	3.883	874	884	910	rBV	57140	164849	41.59%	5.874%
8	4.349	1011	1029	1052	rBV2	53148	138444	34.92%	4.933%
9	5.047	1231	1246	1272	rBV2	114426	293301	73.99%	10.451%
10	5.619	1413	1424	1451	rBV	115360	235725	59.47%	8.399%
11	5.915	1505	1516	1531	rVB7	4691	9690	2.44%	0.345%
12	6.072	1548	1565	1586	rBV	73700	150930	38.07%	5.378%
13	6.992	1840	1851	1869	rBV2	23994	44790	11.30%	1.596%
14	7.320	1938	1953	1972	rBV	118451	210065	52.99%	7.485%
15	7.629	2039	2049	2064	rBV3	14699	25953	6.55%	0.925%
16	8.092	2182	2193	2227	rBV2	200491	396404	100.00%	14.124%
17	8.854	2420	2430	2451	rBV	176363	291035	73.42%	10.370%
18	10.217	2842	2854	2866	rBV	61067	96543	24.35%	3.440%
19	11.156	3137	3146	3156	rBV5	4563	7130	1.80%	0.254%
20	11.252	3164	3176	3200	rBV	175242	273405	68.97%	9.742%
21	11.532	3254	3263	3277	rBV3	10378	17984	4.54%	0.641%
22	11.625	3280	3292	3311	rVV	140241	223299	56.33%	7.956%
23	12.349	3508	3517	3526	rVB6	8974	13342	3.37%	0.475%




Sum of corrected areas: 2806520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022605.D
Acq On : 06 Oct 2021 06:14
Operator : SY/MD
Sample : M4050-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

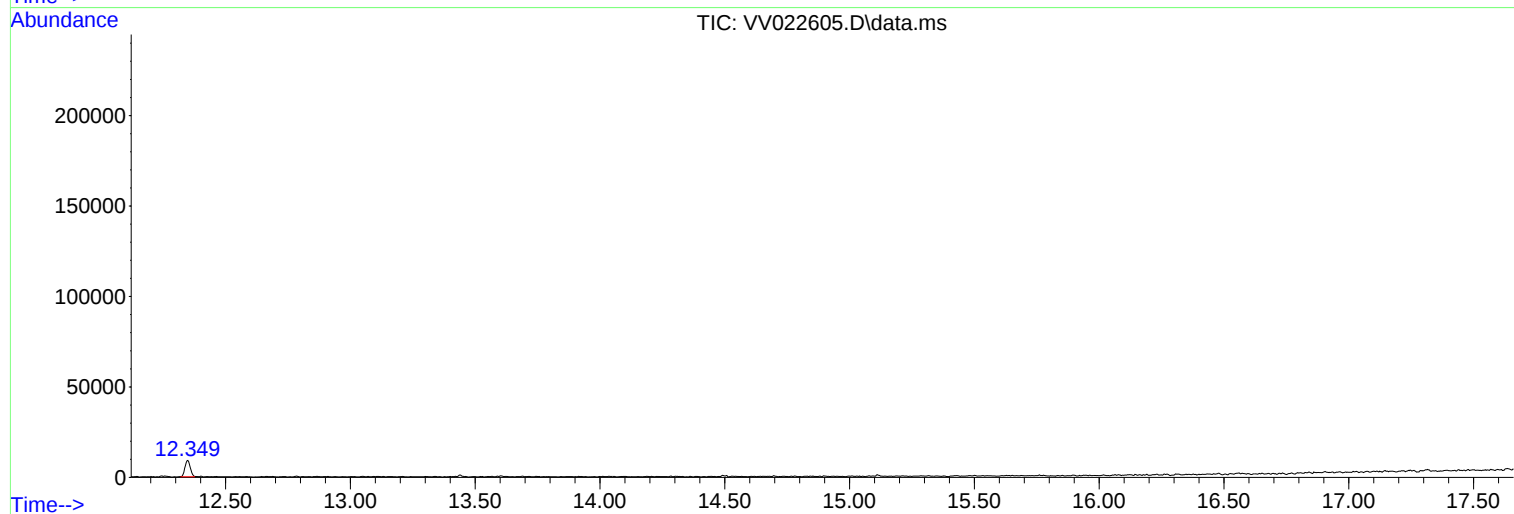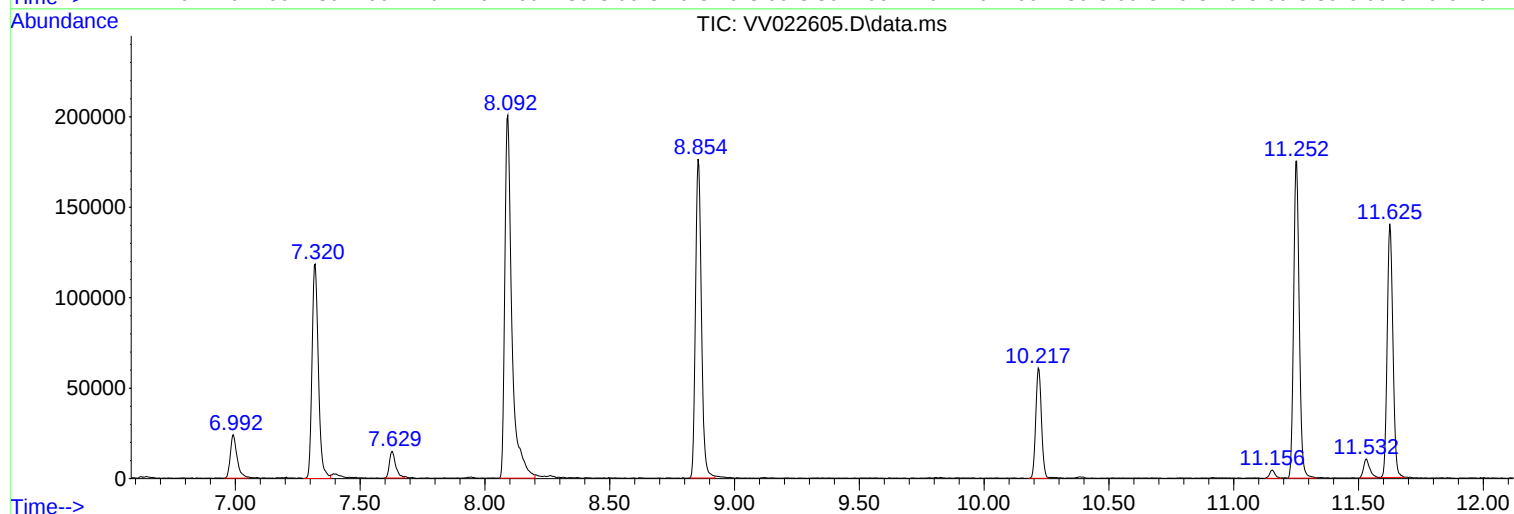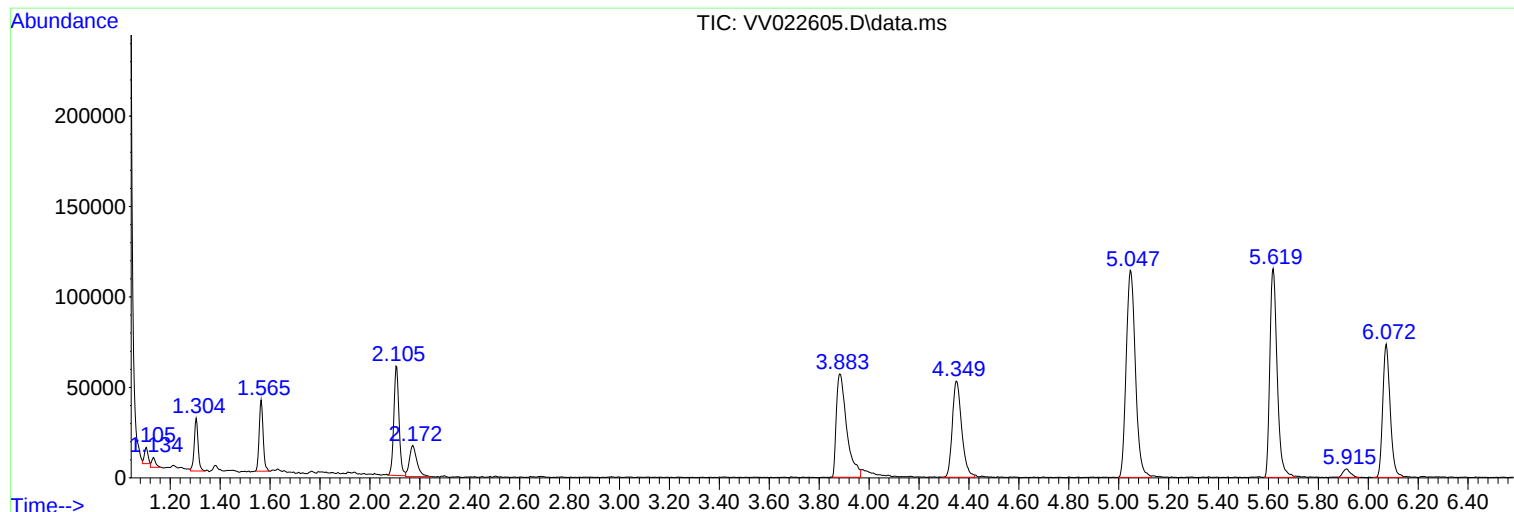

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022605.D
Acq On : 06 Oct 2021 06:14
Operator : SY/MD
Sample : M4050-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022605.D
Acq On : 06 Oct 2021 06:14
Operator : SY/MD
Sample : M4050-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7C6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
