

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022606.D
 Acq On : 06 Oct 2021 06:39
 Operator : SY/MD
 Sample : M4052-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX8

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	62195	63043	9.60%	1.632%
2	1.564	155	163	174	rBV	56694	62771	9.56%	1.625%
3	2.108	321	332	346	rBV2	111943	170234	25.93%	4.406%
4	3.902	874	890	921	rBV3	59095	218587	33.29%	5.657%
5	4.352	1014	1030	1053	rBV2	63722	173850	26.48%	4.499%
6	4.831	1166	1179	1191	rBV4	3786	8236	1.25%	0.213%
7	5.050	1230	1247	1268	rBV2	152714	379098	57.74%	9.811%
8	5.619	1412	1424	1452	rBV	110474	227266	34.61%	5.882%
9	5.915	1503	1516	1541	rBV	334813	656577	100.00%	16.992%
10	6.072	1552	1565	1583	rBV	86979	177843	27.09%	4.603%
11	6.989	1840	1850	1874	rBV	31973	59819	9.11%	1.548%
12	7.317	1941	1952	1970	rBV	175251	309203	47.09%	8.002%
13	7.625	2036	2048	2067	rBV	19284	35594	5.42%	0.921%
14	7.979	2148	2158	2171	rVB2	21910	38034	5.79%	0.984%
15	8.091	2179	2193	2223	rBV2	192351	376713	57.38%	9.749%
16	8.853	2419	2430	2452	rBV	172302	284297	43.30%	7.358%
17	10.217	2843	2854	2868	rBV	62538	99274	15.12%	2.569%
18	11.252	3165	3176	3191	rBV	162905	253244	38.57%	6.554%
19	11.625	3281	3292	3308	rBV	169850	270334	41.17%	6.996%




Sum of corrected areas: 3864017

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022606.D
Acq On : 06 Oct 2021 06:39
Operator : SY/MD
Sample : M4052-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

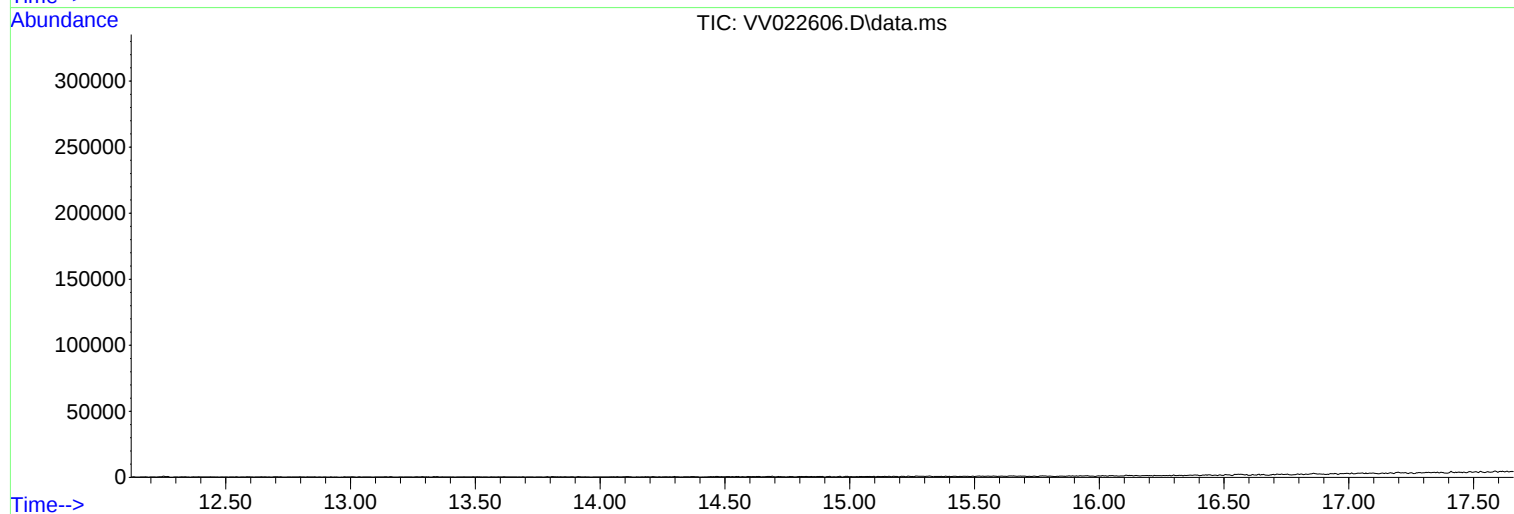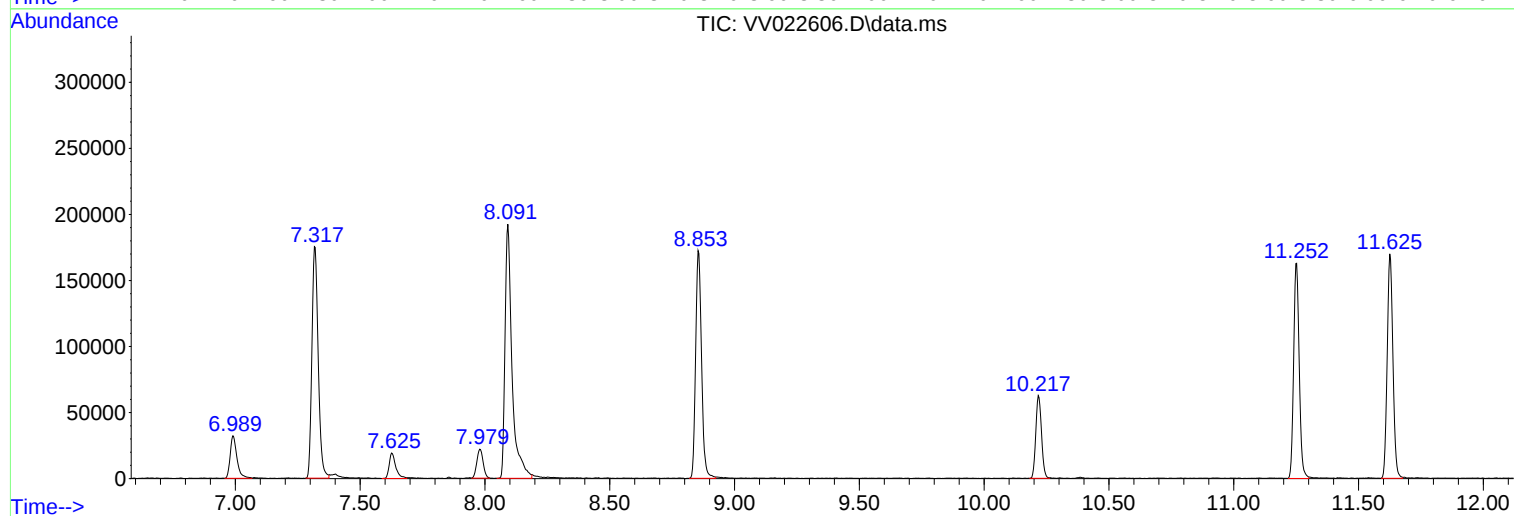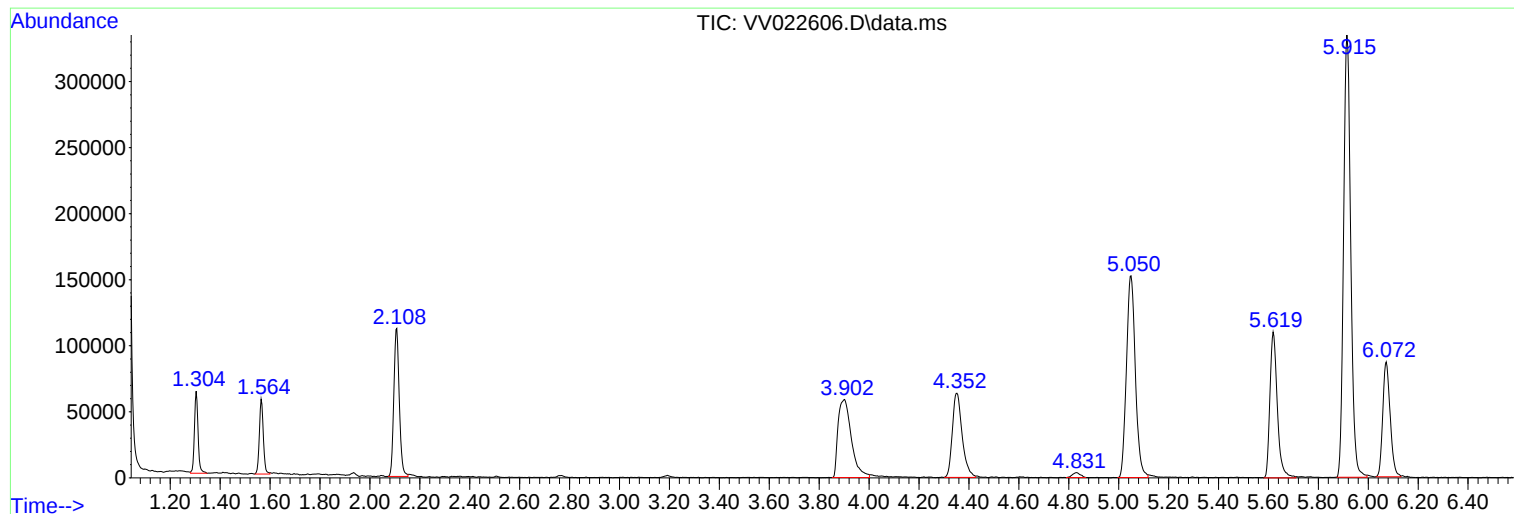

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022606.D
Acq On : 06 Oct 2021 06:39
Operator : SY/MD
Sample : M4052-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022606.D
Acq On : 06 Oct 2021 06:39
Operator : SY/MD
Sample : M4052-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
