

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022607.D
 Acq On : 06 Oct 2021 07:03
 Operator : SY/MD
 Sample : M4052-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB	58836	59904	10.63%	1.356%
2	1.564	151	163	176	rBV	55393	66915	11.88%	1.515%
3	2.108	320	332	348	rBV2	161309	270489	48.02%	6.123%
4	3.188	658	668	680	rVB3	3337	6562	1.16%	0.149%
5	3.908	880	892	914	rBV2	74015	226217	40.16%	5.121%
6	4.349	1010	1029	1056	rBV	67539	174538	30.99%	3.951%
7	4.609	1097	1110	1125	rVB5	3855	8941	1.59%	0.202%
8	5.047	1230	1246	1269	rBV2	157749	381219	67.68%	8.629%
9	5.619	1408	1424	1447	rBV	111404	227586	40.40%	5.152%
10	5.915	1503	1516	1543	rBV	264340	528071	93.75%	11.953%
11	6.072	1552	1565	1592	rVB2	88436	180468	32.04%	4.085%
12	6.989	1841	1850	1866	rBV	32647	59190	10.51%	1.340%
13	7.317	1940	1952	1972	rBV	180035	314946	55.91%	7.129%
14	7.394	1973	1976	1992	rVB3	4279	7206	1.28%	0.163%
15	7.625	2038	2048	2066	rBV	19647	36620	6.50%	0.829%
16	7.976	2144	2157	2181	rBV	336575	563286	100.00%	12.751%
17	8.095	2184	2194	2229	rBV2	179126	396771	70.44%	8.981%
18	8.854	2419	2430	2449	rBV	172633	281958	50.06%	6.382%
19	10.220	2844	2855	2869	rBV	64029	100626	17.86%	2.278%
20	11.252	3164	3176	3193	rBV	162651	254604	45.20%	5.763%
21	11.625	3281	3292	3313	rBV	171977	271598	48.22%	6.148%




Sum of corrected areas: 4417715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022607.D
Acq On : 06 Oct 2021 07:03
Operator : SY/MD
Sample : M4052-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

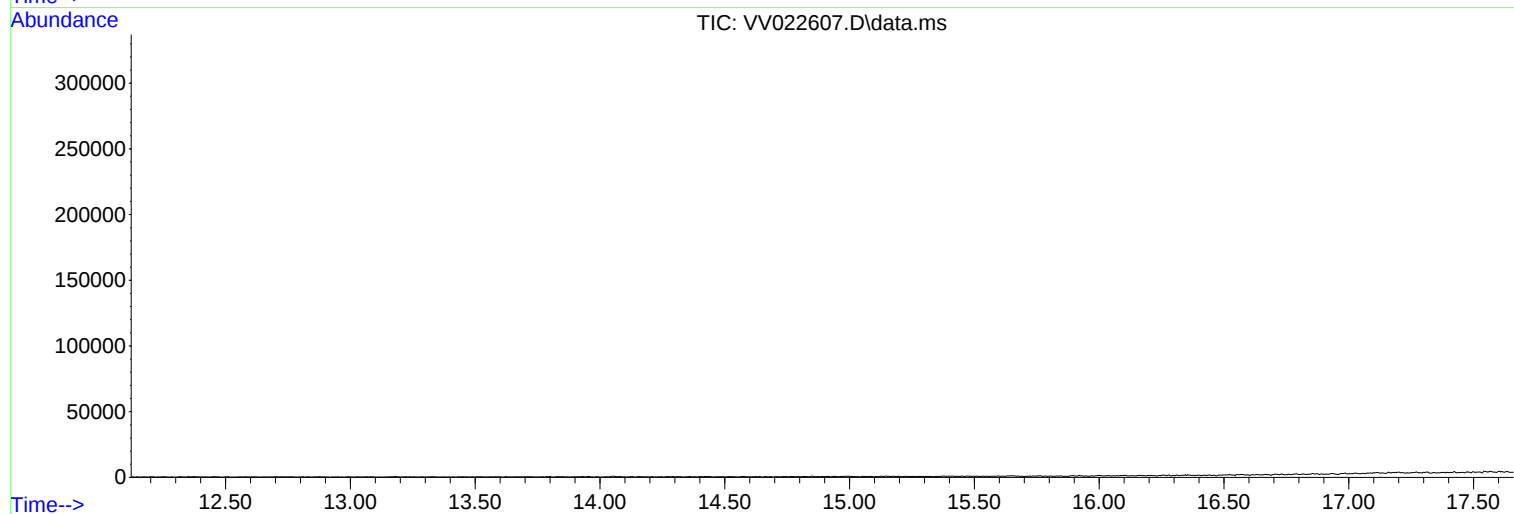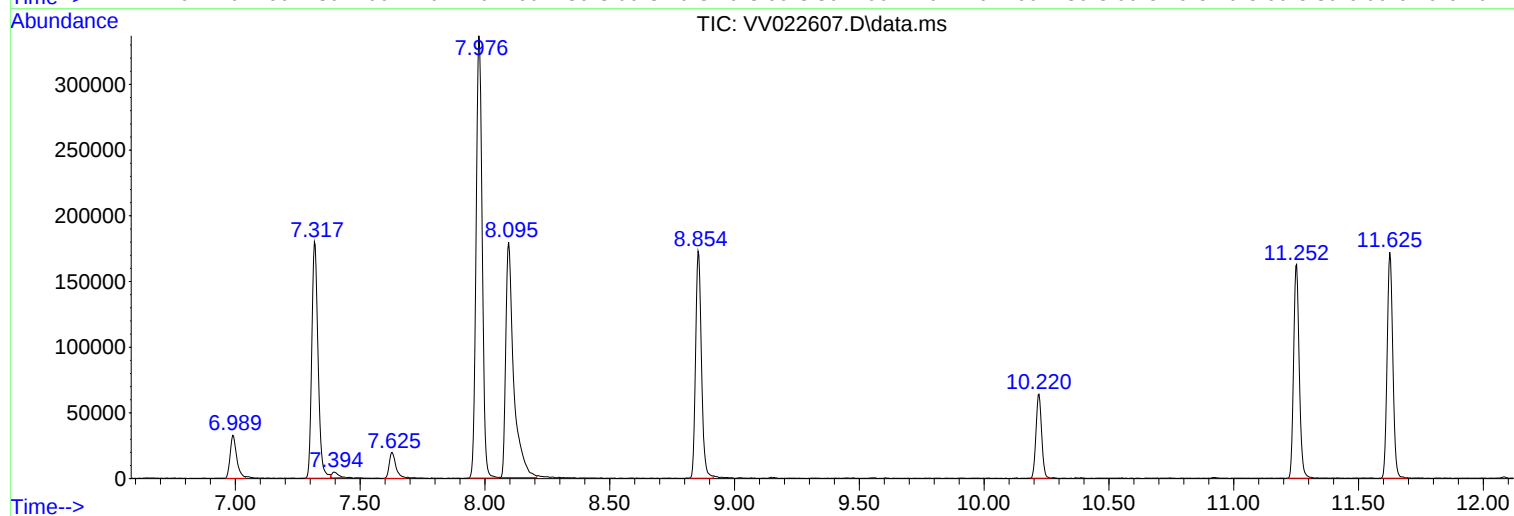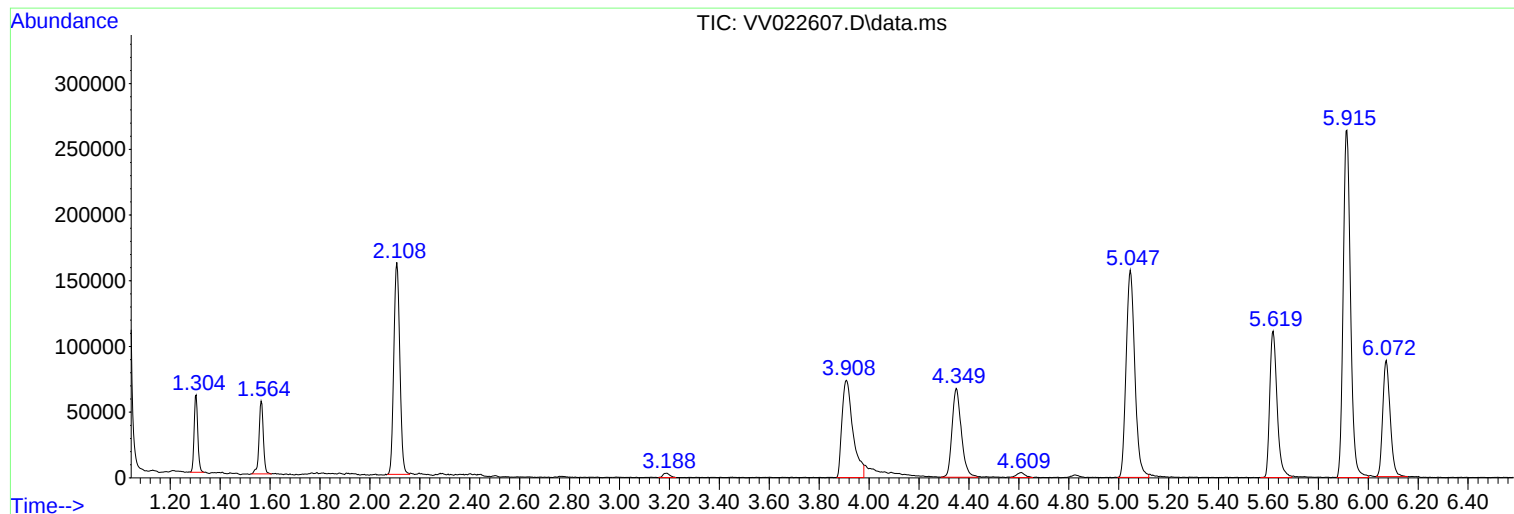

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022607.D
Acq On : 06 Oct 2021 07:03
Operator : SY/MD
Sample : M4052-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
Data File : VV022607.D
Acq On : 06 Oct 2021 07:03
Operator : SY/MD
Sample : M4052-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
