
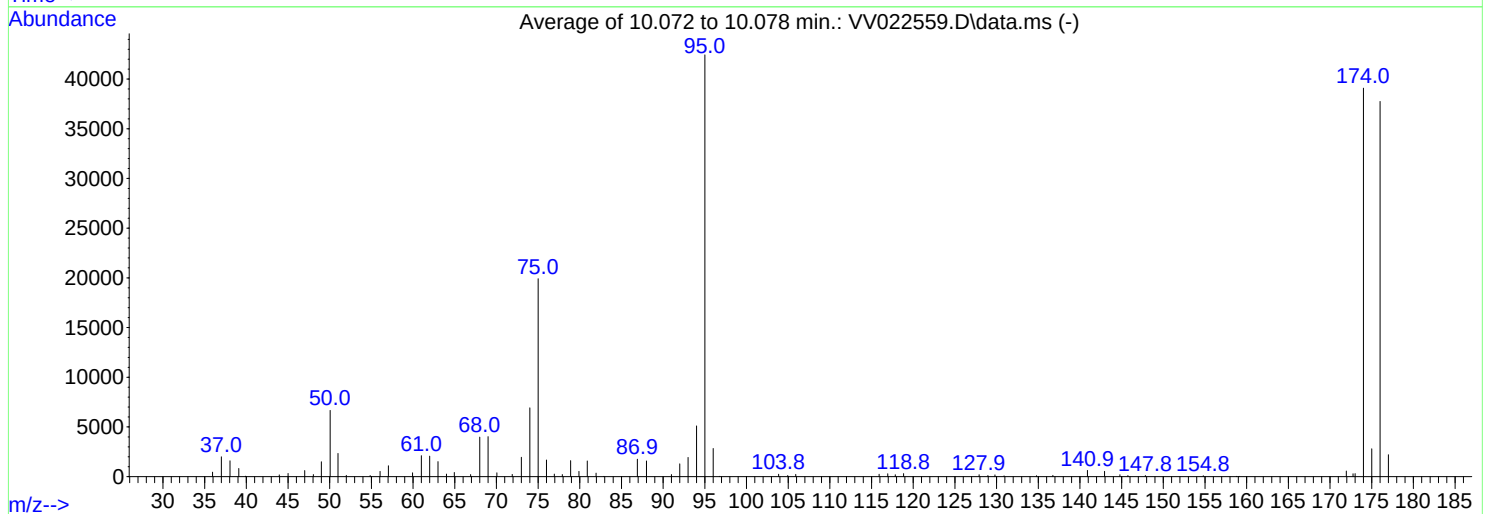


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100521\
 Data File : VV022559.D
 Acq On : 05 Oct 2021 09:12
 Operator : SY/MD
 Sample : BFB209
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB209

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Oct 07 07:45:03 2021

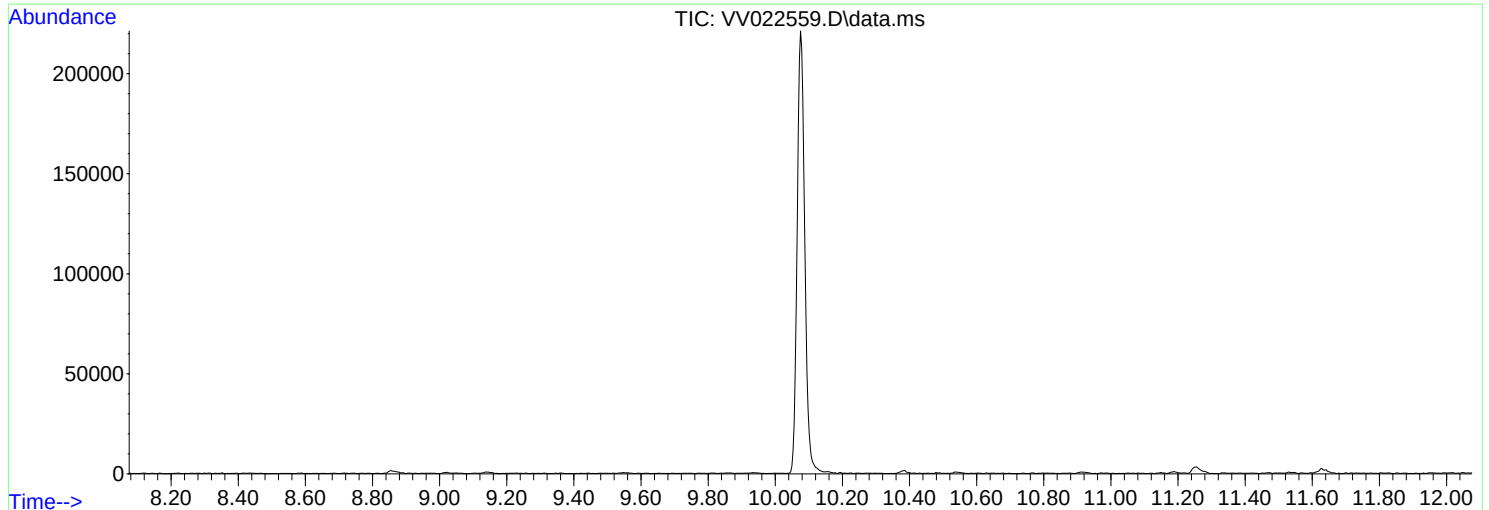

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	6673	PASS
75	95	30	80	46.9	19909	PASS
95	95	100	100	100.0	42437	PASS
96	95	5	9	6.7	2830	PASS
173	174	0.00	2	0.8	315	PASS
174	95	50	120	92.1	39091	PASS
175	174	5	9	7.2	2809	PASS
176	174	95	105	96.6	37757	PASS
177	176	5	10	5.8	2201	PASS

m/z	Abundance
36.00	506.0
37.00	1812.0
38.00	1559.0
39.10	757.0
40.00	159.0
44.00	353.0
45.00	293.0
47.00	524.0
47.90	191.0
49.00	1394.0
50.10	6500.0
51.00	2310.0
51.90	120.0
54.80	113.0
56.10	468.0
57.00	1038.0
59.90	405.0
61.00	1915.0
62.00	1984.0
63.00	1405.0
64.00	267.0
65.00	421.0
66.90	178.0
68.00	3855.0
69.00	4041.0
70.10	405.0
71.90	237.0
73.00	1936.0
74.00	6988.0
75.00	19328.0
76.00	1639.0
77.00	241.0
77.90	244.0
78.90	1542.0
79.90	508.0
80.90	1602.0
81.90	385.0
86.90	1721.0
88.00	1492.0
90.90	216.0
92.00	1264.0
93.00	2052.0
94.00	5049.0
95.00	41944.0
96.00	2673.0
96.80	106.0
103.80	250.0
104.90	100.0
105.90	250.0
115.90	243.0
117.00	338.0
117.80	205.0
118.80	322.0
127.90	189.0
128.90	122.0
129.80	164.0
130.90	111.0
136.80	140.0
140.90	645.0
142.90	502.0
144.80	219.0
145.70	105.0
147.80	119.0
158.80	103.0
171.90	600.0
173.00	502.0
174.00	40096.0
175.00	2735.0
176.00	38200.0
177.00	2283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
39.90	120.0
43.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
35.90	401.0
37.00	2076.0
38.10	1572.0
39.10	863.0
39.90	181.0
44.00	332.0
45.00	335.0
47.00	669.0
48.10	223.0
49.00	1555.0
50.00	6650.0
51.00	2301.0
52.10	145.0
54.90	100.0
56.00	581.0
57.10	1137.0
60.00	365.0
61.00	2194.0
62.00	2046.0
63.00	1575.0
64.00	244.0
64.90	390.0
66.90	210.0
68.00	3944.0
69.00	3930.0
70.00	356.0
71.90	223.0
73.00	1916.0
74.00	6657.0
75.00	19824.0
76.00	1633.0
76.90	249.0
77.90	163.0
78.90	1649.0
79.90	538.0
80.90	1475.0
82.00	310.0
82.90	107.0
86.90	1767.0
88.00	1645.0
91.10	203.0
92.00	1299.0
93.00	1710.0
94.00	5024.0
95.00	41256.0
96.00	2903.0
103.90	235.0
105.00	115.0
105.90	198.0
115.90	226.0
116.90	248.0
117.90	188.0
118.90	282.0
127.90	191.0
129.00	104.0
129.80	167.0
134.80	149.0
136.80	115.0
140.90	590.0
143.00	555.0
144.80	152.0
145.90	116.0
147.90	108.0
154.80	172.0
159.10	107.0
172.00	511.0
172.70	425.0
174.00	36672.0
175.00	2812.0
176.00	36096.0
177.00	2042.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	438.0
37.00	2081.0
38.10	1644.0
39.10	844.0
39.90	175.0
44.00	328.0
45.00	341.0
47.00	637.0
48.10	210.0
49.00	1553.0
50.00	6870.0
51.00	2391.0
52.00	128.0
54.80	116.0
56.10	525.0
57.00	1119.0
59.90	400.0
61.00	2218.0
62.00	2162.0
63.00	1567.0
64.00	253.0
65.00	428.0
66.90	217.0
68.00	4110.0
69.00	4129.0
70.00	413.0
71.90	216.0
73.00	2009.0
74.00	7142.0
75.00	20576.0
76.00	1749.0
76.90	279.0
77.90	217.0
78.90	1642.0
79.90	558.0
80.90	1639.0
81.90	352.0
86.90	1796.0
88.00	1620.0
91.00	229.0
92.00	1307.0
93.00	2015.0
94.00	5255.0
95.00	44112.0
96.00	2915.0
103.90	252.0
105.00	112.0
105.90	227.0
115.90	250.0
116.90	285.0
117.80	194.0
118.90	325.0
127.90	201.0
129.00	125.0
129.80	186.0
130.90	119.0
134.80	142.0
136.70	138.0
140.90	645.0
142.90	514.0
144.80	202.0
145.70	119.0
147.90	126.0
154.80	141.0
171.90	568.0
172.80	470.0
173.00	444.0
174.00	40504.0
175.00	2880.0
176.00	38976.0
177.00	2279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209