

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100523\
 Data File : VW032264.D
 Acq On : 05 Oct 2023 18:36
 Operator : SY/MD
 Sample : 04748-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX885

Quant Time: Oct 06 01:31:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 06 01:20:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	81570	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	85286	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	38499	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	29815	4.494	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.800%
7) Chloroethane-d5	1.535	69	27820	5.166	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.400%
11) 1,1-Dichloroethene-d2	2.063	65	12405	4.434	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.600%
20) 2-Butanone-d5	3.796	46	90939	54.189	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.380%
24) Chloroform-d	4.256	84	60356	5.157	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	4.950	65	30092	5.428	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.600%
32) Benzene-d6	4.966	84	115052	4.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	5.995	67	39278	4.724	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.400%
41) Toluene-d8	7.249	98	101961	4.443	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	7.561	79	13431	4.559	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.030	63	71613	51.659	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.320%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	30811	5.298	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.000%
66) 1,2-Dichlorobenzene-d4	11.564	152	37740	5.283	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.600%
Target Compounds						Qvalue
13) Acetone	2.127	43	2226	1.721	ug/L	90
18) trans-1,2-Dichloroethene	2.699	96	12248	1.787	ug/L	97
22) cis-1,2-Dichloroethene	3.822	96	12373	1.677	ug/L	95
25) Chloroform	4.285	83	21307	1.685	ug/L	97
31) Carbon tetrachloride	4.738	117	151329	15.424	ug/L	98
34) Trichloroethene	5.838	95	50375	6.145	ug/L	98
35) Methylcyclohexane	6.053	83	3908	0.308	ug/L #	73
42) Toluene	7.326	91	8162	0.255	ug/L	99
52) Ethylbenzene	8.960	91	2682	0.075	ug/L	98
53) m,p-Xylene	9.085	106	1960	0.148	ug/L	91
63) 1,2,4-Trimethylbenzene	10.857	105	2253	0.093	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100523\
Data File : VV032264.D
Acq On : 05 Oct 2023 18:36
Operator : SY/MD
Sample : 04748-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX885

Quant Time: Oct 06 01:31:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 06 01:20:04 2023
Response via : Initial Calibration

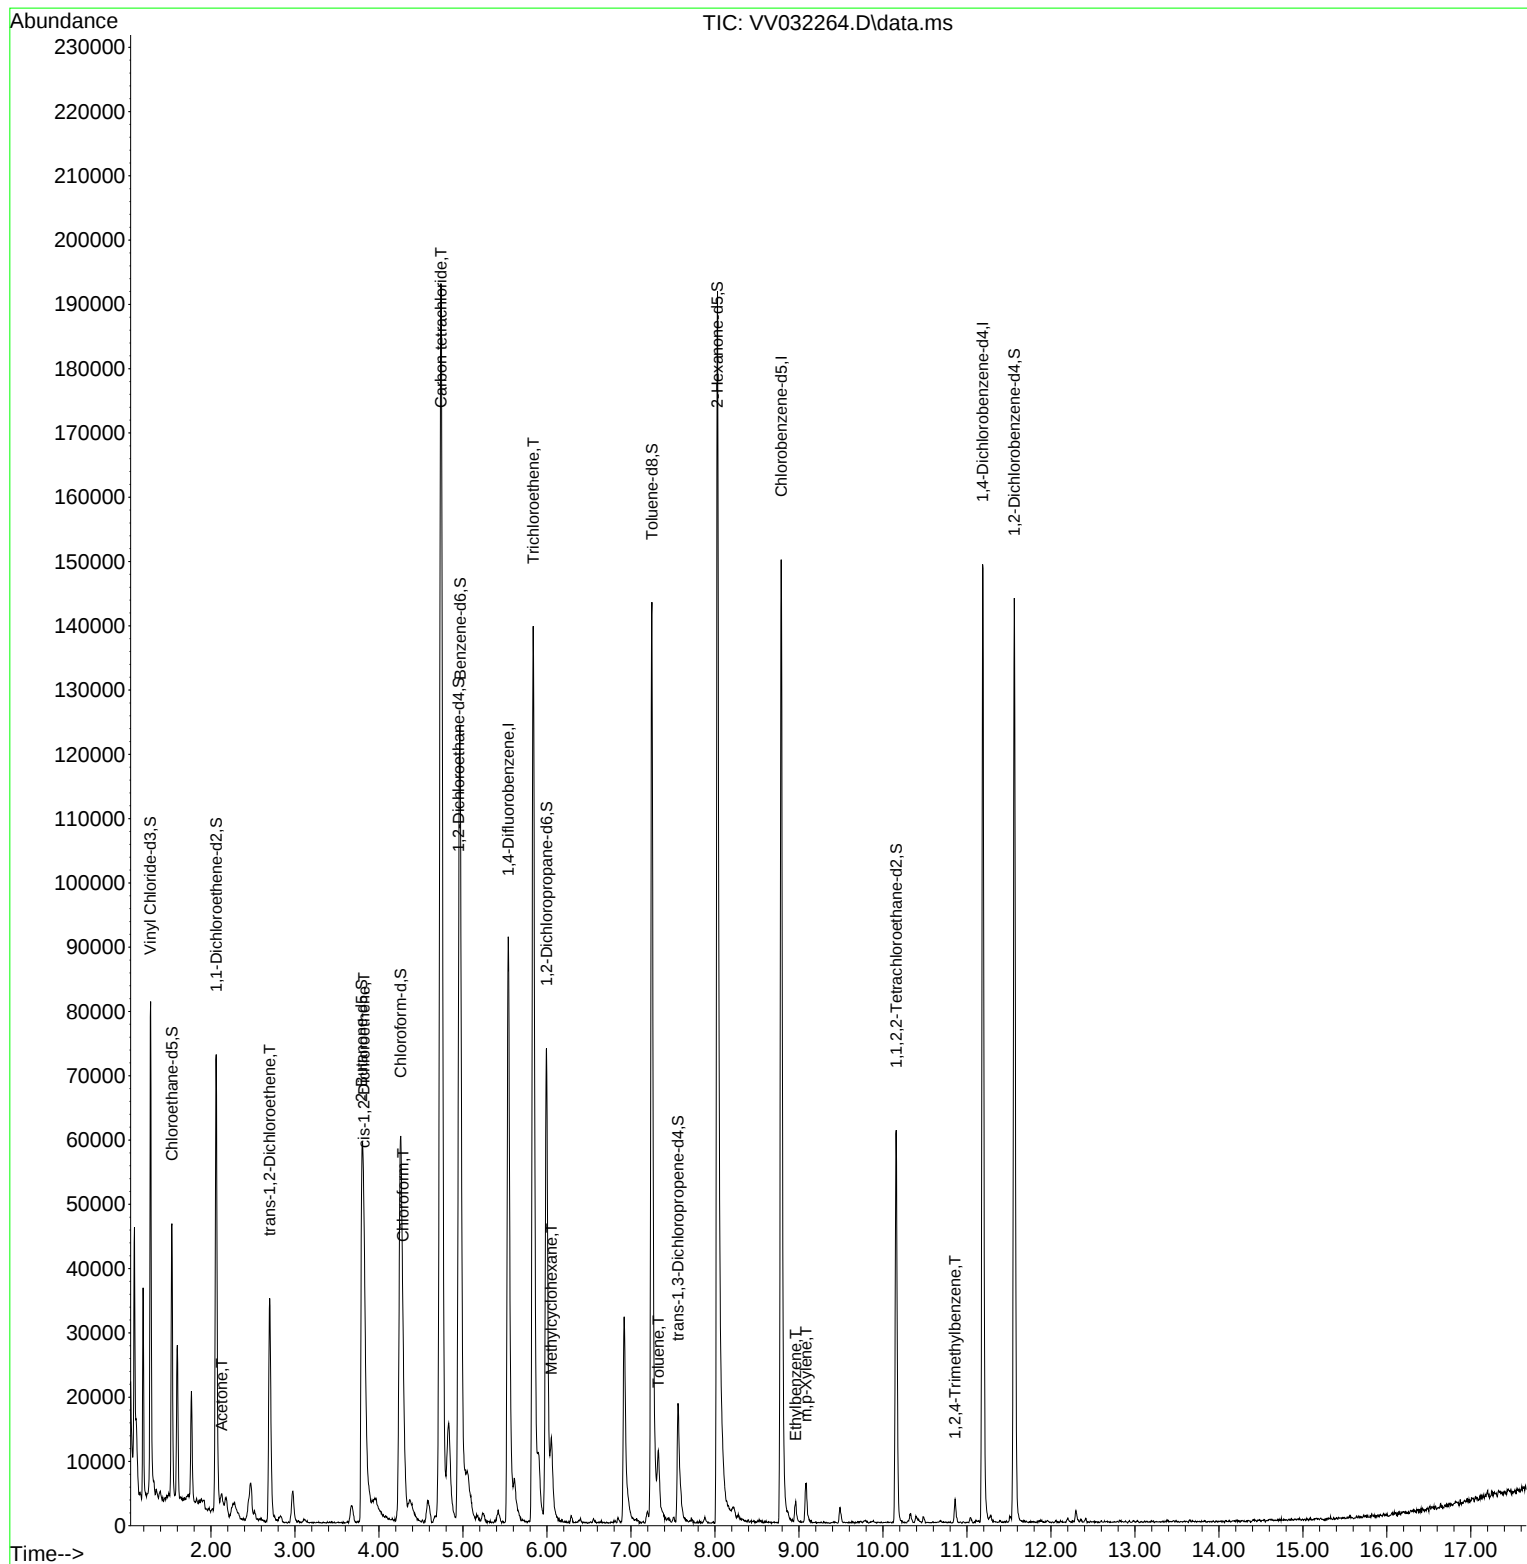

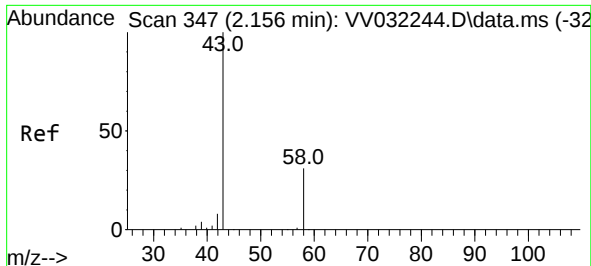

#13

Acetone

Concen: 1.721 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.029 min

Lab File: VV032264.D

Acq: 05 Oct 2023 18:36

Instrument :

MSVOA_V

ClientSampleId :





EX885

Tgt Ion: 43 Resp: 2226

Ion Ratio Lower Upper

43 100

58 38.7 0.0 66.0

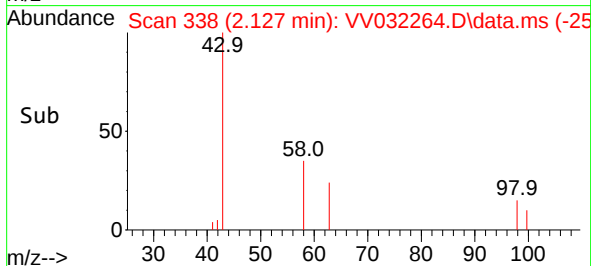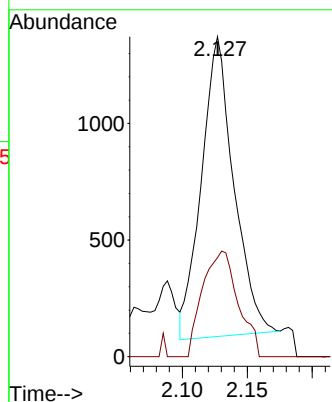

#18

trans-1,2-Dichloroethene

Concen: 1.787 ug/L

RT: 2.699 min Scan# 516

Delta R.T. 0.006 min

Lab File: VV032264.D

Acq: 05 Oct 2023 18:36




Tgt Ion: 96 Resp: 12248


Ion Ratio Lower Upper

96 100

61 133.8 96.9 180.1

98 63.9 45.3 84.1


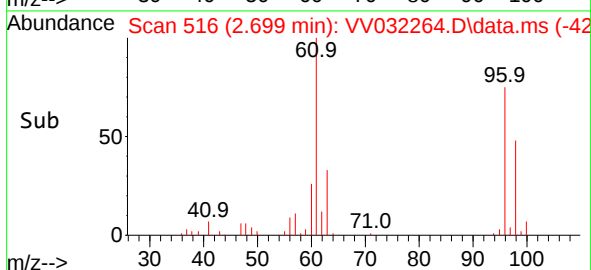
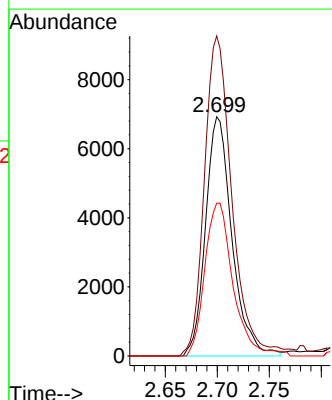
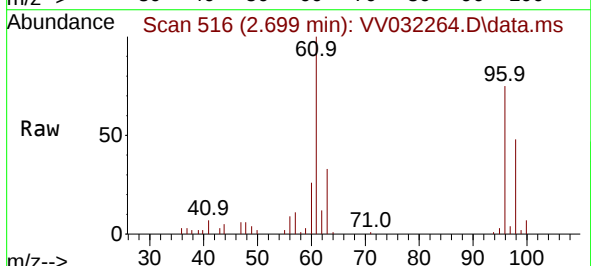




#22
cis-1,2-Dichloroethene
Concen: 1.677 ug/L
RT: 3.822 min Scan# 80
Delta R.T. 0.003 min
Lab File: VV032264.D
Acq: 05 Oct 2023 18:36




Instrument :
MSVOA_V
ClientSampleId :
EX885


Tgt Ion: 96 Resp: 12373
Ion Ratio Lower Upper
96 100
61 114.6 85.8 159.4
98 63.1 44.0 81.6

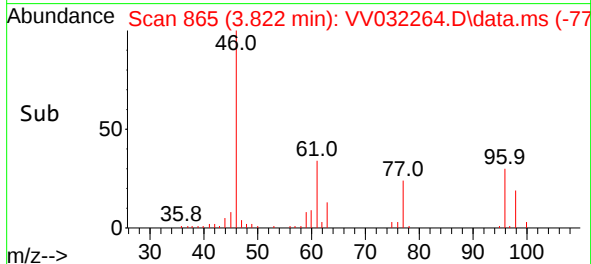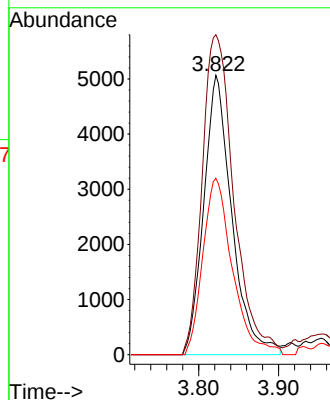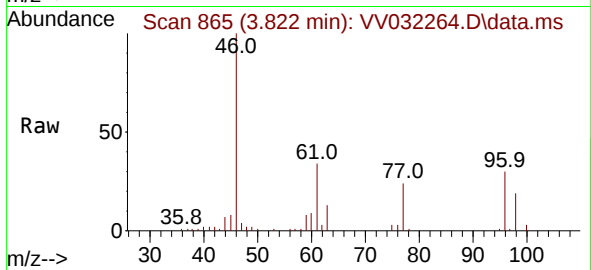

#25
Chloroform
Concen: 1.685 ug/L
RT: 4.285 min Scan# 1009
Delta R.T. 0.006 min
Lab File: VV032264.D
Acq: 05 Oct 2023 18:36

Tgt Ion: 83 Resp: 21307
Ion Ratio Lower Upper
83 100
85 62.3 45.4 84.4



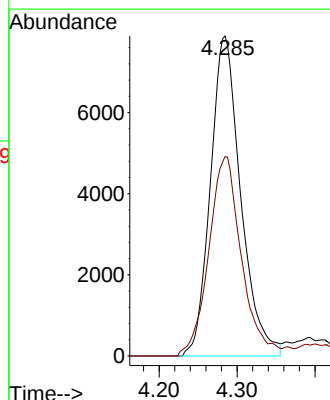
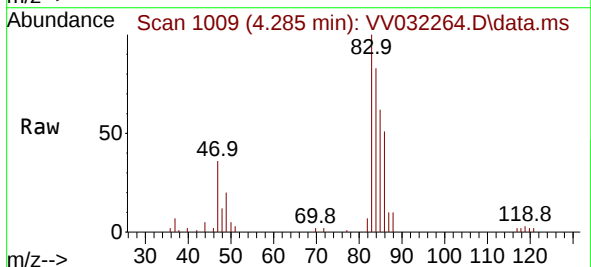




#31
Carbon tetrachloride
Concen: 15.424 ug/L
RT: 4.738 min Scan# 1150
Delta R.T. 0.000 min
Lab File: VV032264.D
Acq: 05 Oct 2023 18:36




Instrument :
MSVOA_V
ClientSampleId :
EX885


Tgt Ion:117 Resp: 151329
Ion Ratio Lower Upper
117 100
119 94.8 77.6 116.4

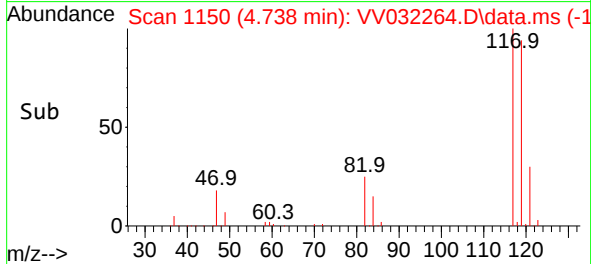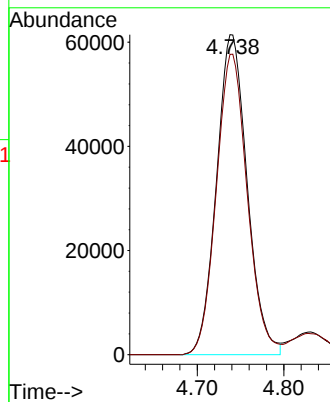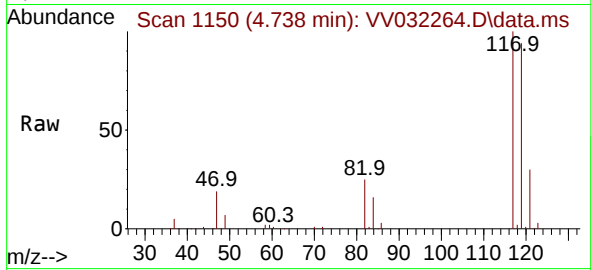

#34
Trichloroethene
Concen: 6.145 ug/L
RT: 5.838 min Scan# 1492
Delta R.T. 0.003 min
Lab File: VV032264.D
Acq: 05 Oct 2023 18:36

Tgt Ion: 95 Resp: 50375
Ion Ratio Lower Upper
95 100
97 66.0 45.7 84.9
132 97.6 70.3 130.5
130 101.5 69.6 129.2

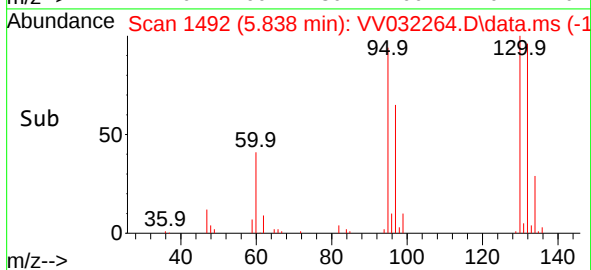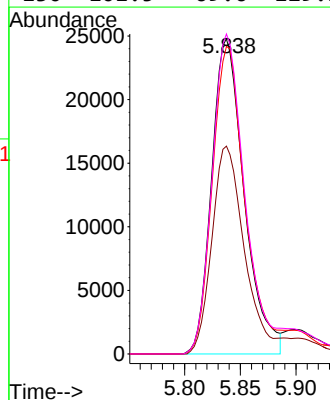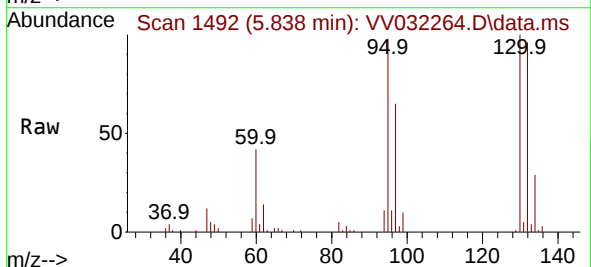

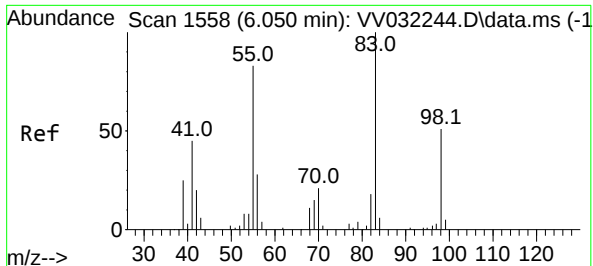

#35

Methylcyclohexane

Concen: 0.308 ug/L

RT: 6.053 min Scan# 1559

Delta R.T. 0.003 min

Lab File: VV032264.D

Acq: 05 Oct 2023 18:36

Instrument :

MSVOA_V

ClientSampleId :

EX885





Tgt Ion: 83 Resp: 3908

Ion Ratio Lower Upper

83 100

55 55.8 64.2 96.2#

98 31.4 39.6 59.4#

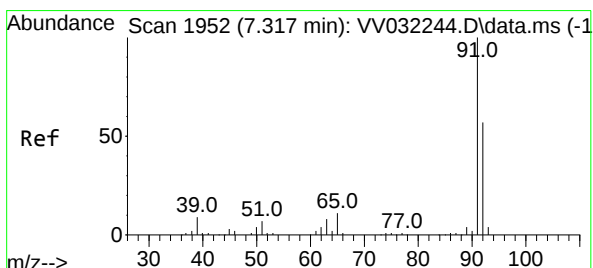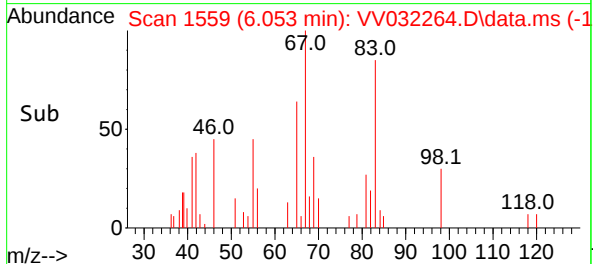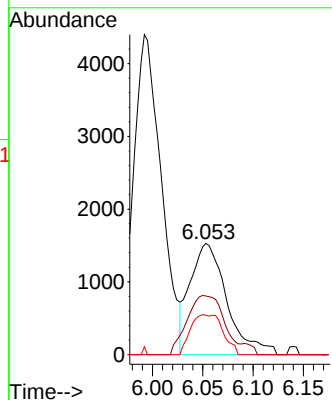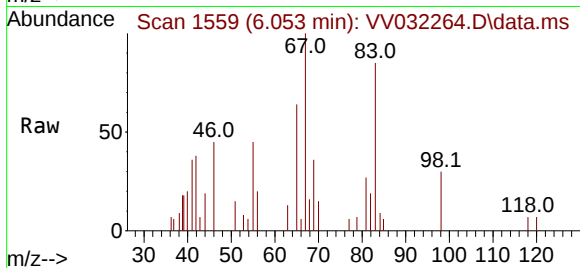

#42

Toluene

Concen: 0.255 ug/L

RT: 7.326 min Scan# 1955

Delta R.T. 0.010 min

Lab File: VV032264.D




Acq: 05 Oct 2023 18:36


Tgt Ion: 91 Resp: 8162

Ion Ratio Lower Upper

91 100

92 57.2 40.8 75.8


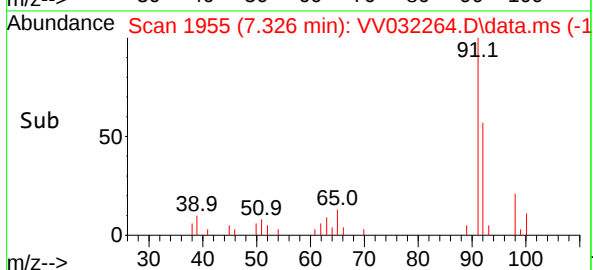
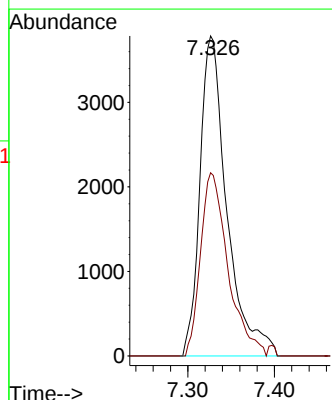
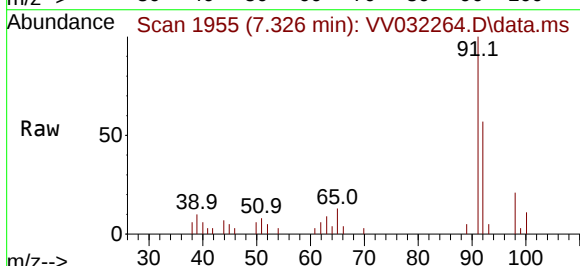




#52
Ethylbenzene
Concen: 0.075 ug/L
RT: 8.960 min Scan# 2460
Delta R.T. 0.010 min
Lab File: VV032264.D
Acq: 05 Oct 2023 18:36




Instrument :
MSVOA_V
ClientSampleId :
EX885


Tgt Ion: 91 Resp: 2682
Ion Ratio Lower Upper
91 100
106 31.2 21.3 39.5

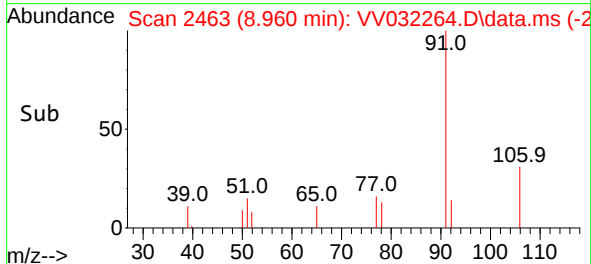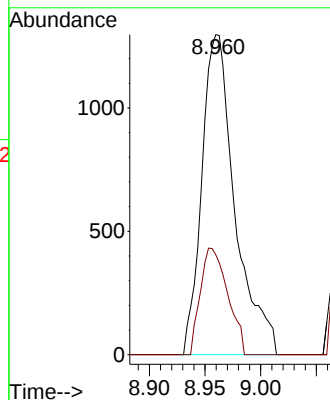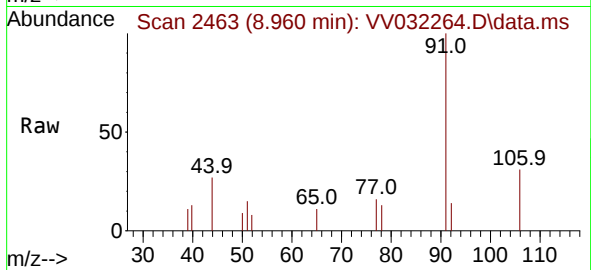

#53
m,p-Xylene
Concen: 0.148 ug/L
RT: 9.085 min Scan# 2502
Delta R.T. 0.010 min
Lab File: VV032264.D
Acq: 05 Oct 2023 18:36

Tgt Ion: 106 Resp: 1960
Ion Ratio Lower Upper
106 100
91 220.5 144.5 268.3

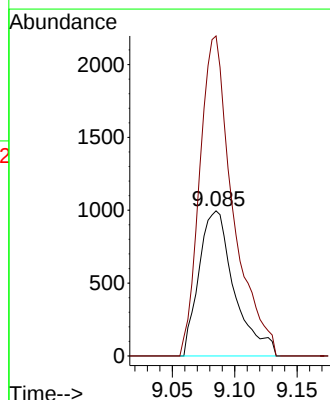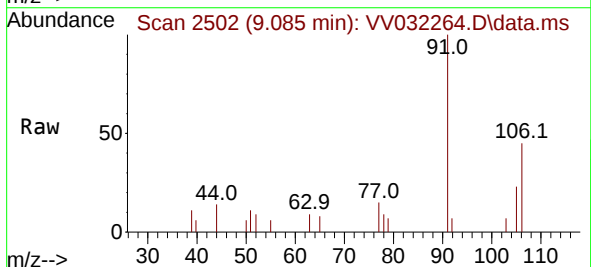



#63
 1,2,4-Trimethylbenzene
 Concen: 0.093 ug/L
 RT: 10.857 min Scan# 3053
 Delta R.T. 0.003 min
 Lab File: VV032264.D
 Acq: 05 Oct 2023 18:36

Instrument :
 MSVOA_V
 ClientSampleId :
 EX885

Tgt Ion:105 Resp: 2253
 Ion Ratio Lower Upper
 105 100
 120 46.9 36.2 54.4

